

# REFERENCE MATERIAL CERTIFICATE

## ISO 17034

### **Certified Reference Material**

This certificate is designed in accordance with ISO 17034 and ISO Guide 31. This certified reference material (CRM) was designed, produced and verified in accordance with ISO/IEC 17025, ISO 17034 and a registered quality management system ISO 9001.

Product Name	Product Code	Lot Number	Format	Expiry Date	Storage Temp
Canada Pesticide Mixture 4 ver. 2 20-500 µg/mL in	DRE-A50000074AL	2-H389602AL	Multicomponent Solution	31 Oct 2021	≤ -10 ºC
Acetonitrile					


Compound Name	CERTIF Concentration (mg/L)	Expanded Uncertainty U ( mg/L )	CAS	Lot Number	Combined Purity (%)	Amount (mg)	RT (min)
Thiophanate Methyl	49.97	2.7	23564-05-8	1862.421.1P	99.94	5.00	12.61
Pentachloronitrobenzene	20.11	1.2	82-68-8	95.7.1.1P	98.6	2.01	17.08
Benzovindiflupyr	20.1	1.1	1072957-71-1	8791.3.2P	99.5	2.01	18.20
Fenpyroximate (mixture Of Raceimers)	19.97	1.1	111812-58-9	2985.286.1P	99	2.00	21.58
Endosulfan I	202	11	959-98-8	266.3.6P	99.5	20.30	21.58
Endosulfan li	50.64	2.7	33213-65-9	253.3.3P	99.3	5.06	22.63
Endosulfan Sulfate	50.49	2.8	1031-07-8	254.421.5P	99	5.05	23.29
Fenoxycarb	20.04	1.1	72490-01-8	1871.421.1P	99.69	2.00	24.15
Bifenazate	19.89	2.2	149877-41-8	2960.421.1P	99.87	1.99	24.16
Permethrin (mixture Of Isomers)	503.6	25	52645-53-1	1184.421.4.2P	97.79	51.50	25.64
Baythroid (mixture Four Of Isomers)	202	11	68359-37-5	1067.3.10.1P	97.6	20.70	26.02
Acequinocyl	30.05	1.6	57960-19-7	2868.3.3P	99.5	3.00	26.44
Fenvalerate (mixture Of Diastereoisomers)	100.3	6	51630-58-1	1623.421.1P	98.37	10.20	26.93
Deltamethrin	503.6	26	52918-63-5	1622.421.4.2P	99.73	50.50	27.59

The producer certifies that this reference material meets the specification stated in this certificate until the expiry date, provided it is stored unopened at the recommended temperature herein. Product warranties for this reference material are set out in the	CERTIFIED BY CERTIFIED ON		H-7/ H	RM
terms and conditions of purchase.	HuiChen Stavros, Ph.D.	21 Nov 2019	Murchen Xun	Release



## REFERENCE MATERIAL CERTIFICATE

### ISO 17034

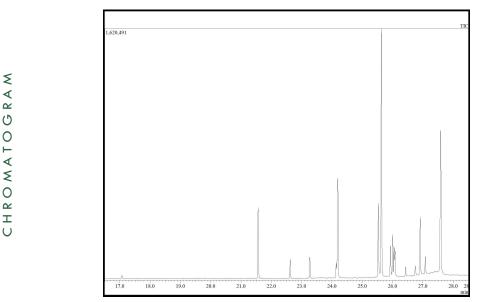

Instrument GC/MS Detection MS Column Phenomenex ZB-Semivolatile 30m x 0.25 mm, ID 0.25 um	Method of Preparation The certified value is based on gravimetric and volumetric preparation of this CRM. This CRM has been confirmed by the appropriate analytical techniques.
Method Details   Rate Temp.(C) Hold time (min)   40.0 2.0   10.0 100.0 0.0   15.0 250.0 0.0   20.0 345.0 3.25	Batch Information Solvent: Acetonitrile, Lot no. 191823, 100 mL
InjVol 1 μl Flow 1 ml/min	permethrin (mixture of isomers) : cis: 24%. trans 76%

#### Intended Use

This CRM is intended for use in a laboratory as a calibration and quality control standard or in method development for analytical techniques.

#### Safety

Proper precautions should be observed while handling. See Safety Data Sheet.

#### Uncertainty

The certified value(s) and uncertainty(ies) are determined in accordance with ISO 17034 with an 95% confidence level (k=2). Uncertainty is based on the Total Combined Uncertainty, including uncertainties of preparation, purity of neat materials, homogeneity, long-term stability testing, and transportation stability.

#### Traceability

The balances used for gravimetric measurements are calibrated with weights traceable to the national standards (NIST). The calibration of the balances is verified daily internally and annually by an external accredited calibration service. Only Class A glassware is used for volumetric measurements.

#### Homogeneity

Random replicate samples of the final packaged CRM have been analysed to prove homogeneity consistent with ISO 17034.

#### Storage

The CRM should be stored in the original sealed bottle at the indicated temperature.

#### Instructions for Use

1

The CRM should be used shortly after opening to avoid concentration changes due to evaporation. It is recommended to use 1 µL as the minimum sample size. If storage after opening is necessary, it should be transferred to an amber vial with minimum head space and a Teflon lined silicon septum. If handled as recommended, use period after opening is a maximum of 81 days for an estimated 5% drift in concentration as a result of analyte and/or solvent transpiration. Visit the support section of our website lgcstandards.com for a series of Dr. Ehrenstorfer Tech Tip videos and frequently asked questions.

## LGC Group

7290-B Investment Drive North Charleston, SC 29418 United States T | +1 843 763 4884 F | +1 866 509 5146 E | dr.ehrenstorfer@lgcgroup.com The producer of this reference material is registered to ISO 9001:2015 under IZ391-IS4 by NSF-ISR and accredited to ISO 17025:2005 and ISO 17034:2016 by A2LA with the accreditation numbers 3031.01 and 3031.02.

