

Certificate of Analysis

Reference Substance

Nicotinamide


Catalogue Number: LGCFOR0552.00

 Long-term Storage;

2 to 8 °C, dark

Appearance: white solid
Melting Point: 129 °C

Assay 'as is': 99.8 %

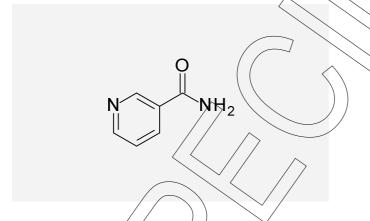

Date of shipment: 2020-November-30

This certificate is valid for two years from the date of shipment provided the substance is stored under the recommended conditions.

Release Date:

2014-01-15

LGC GmbH

Dr. Sabine Schröder Product Release








I. Identity

The identity of the reference substance was established by following analyses.

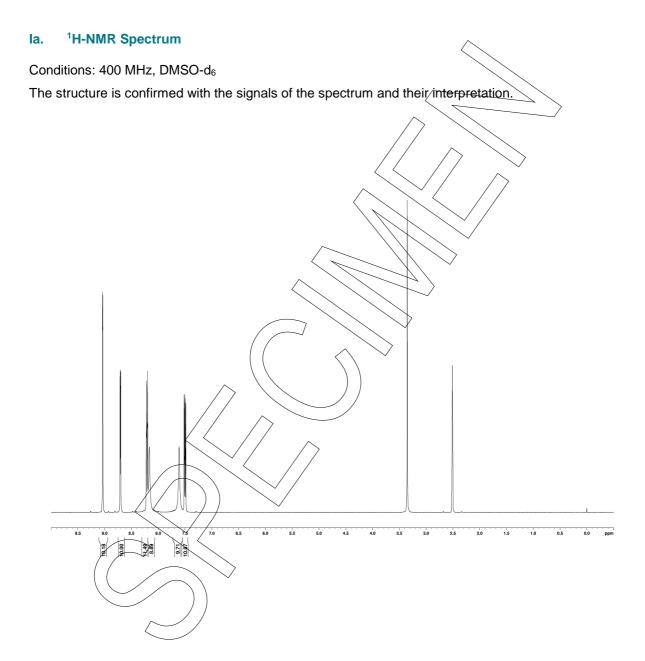






Ib. Mass Spectrum

Method: EI, 70eV, detector temperature: 280 °C

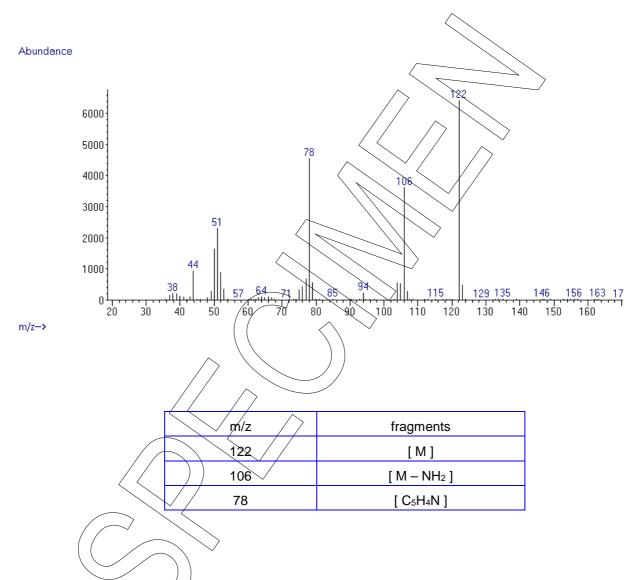


The signals of the mass spectrum and their interpretation are consistent with the structural formula.





Ic. IR Spectrum

Method: Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy

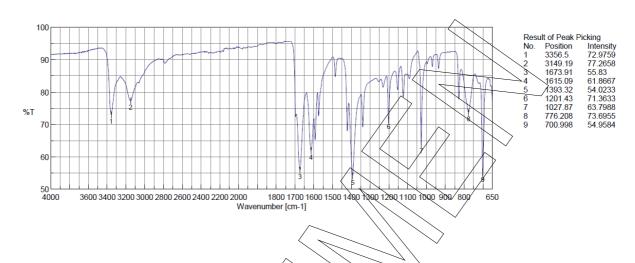

The signals of the IR spectrum and their interpretation are consistent with the structural formula.

II. Purity


The purity of the reference substance was analysed by high performance liquid chromatography (HPLC).

HPLC Conditions:

Column: Detector: Injector: Discovery HS F5 1.0 ml/min, 40 °C DAD Auto 3 μ m, 150 x 4 mm Water/Acetonitrile 15/85 (v/v); 260 nm 5 μ l; 0.06344 mg/ml in Water/Acetonitrile 50/50 (v/v)





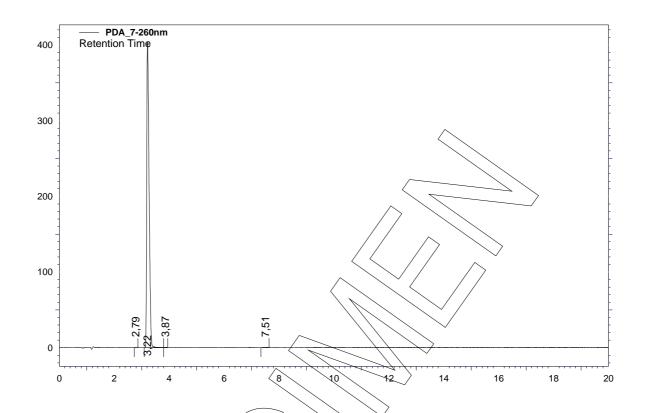

Area Percent Report - Sorted by Signal

Pk#	Retention Time	Area	Area %	
1	2,79/	492	0.02	
2	3.22	2382028	99.92	
3	<3.87 / /	576	0.02	
4	7.51	856	0.04	
Totals		2383952	100.00	

For the calculation the system peaks were ignored. The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %.

Results:





III. Water Content

Method: Karl Fischer titration

Results:

 $\begin{tabular}{lll} Average & 0.08 \% \\ Number of results & n=3 \\ Standard deviation & 0.01 \% \\ \end{tabular}$



Method: 1H-NMR

No significant amounts of residual solvents were detected (< 0.05 %)



Total impurities (HPLC) 0.08 %

Water content 0.08 %

Residual solvents n. d. (not detected)

Assay (100 % method) 1 99.84 %

The assay is assessed to be 99.8 % 'as is'

The assay 'as is' is equivalent to the assay based on the not anhydrous and not dried substance respectively.



Assay (%) = (100 % - KF - RES) * Purity HPLC (%) 100 %

Water (KF) and Residual solvents (RES) are considered as absolute contributions, HPLC purity is considered as relative contribution.

Standards

LGCFOR0552.00 Lot Number 42033

Excellence through measurement