

## Certificate of Analysis

## ISO 17034

### Reference Material

#### Product name

Etidronate Disodium

#### Product code

MM3079.00

#### CAS number

7414-83-7

#### Molecular weight

249.99

#### Molecular formula

C<sub>2</sub>H<sub>6</sub>O<sub>7</sub>P<sub>2</sub> · 2Na

#### Lot number

G1060111

#### Appearance


white solid

#### Melting point

> 285 °C (dec.)

#### Long-term storage

2 to 8 °C, dark  
very hygroscopic

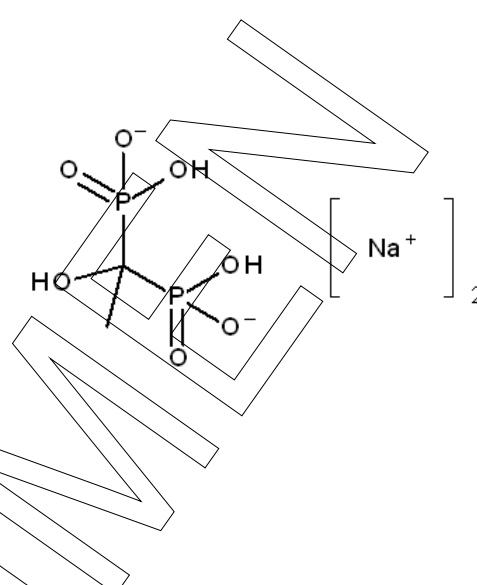

Assay<sup>1</sup> "as is"  
**96.8 %**

Uncertainty<sup>2</sup> U  
**0.4 %**

**Intended Use:** Use for identification and quantification. The assay is verified by a second testing method. Due to the homogeneity studies, the minimum amount of sample to be used is 15 mg.

Date of shipment: **06 Jul 2020**

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **one year** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

<b>Release by:</b>	<b>Date of Release:</b>		Product Release
Dr. Sabine Schröder	Luckenwalde, 17 Jun 2020		

<sup>1</sup> Calibration and verification were carried out using standards traceable to SI-units. The value is expressed on an "as is" basis.

<sup>2</sup> The uncertainty "U" is the expanded uncertainty of the testing method for the assigned value estimated in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM). It corresponds to a level of confidence of about 95%. Coverage factor k = 2.



## Important product information

This RM is intended for laboratory use only and is not suitable for human or animal consumption.

This RM conforms to the characteristics of a primary standard as described in the ICH Guidelines. The values quoted in this Certificate of Analysis are the producer's best estimate of the true values within the stated uncertainties and based on the techniques described in this Certificate of Analysis. The production of this RM was undertaken in accordance with the requirements of ISO 17034. The identity is verified by data from international scientific literature.

## Storage and handling

Before usage of the RM, it should be allowed to warm to room temperature. No drying is required, as assigned values are already corrected for the content of water and other volatile materials.

## Further content

- Assigned value
- Purity
- Identity
- Stability and homogeneity
- Revision table

SPECIMEN



## Assigned value

**Assay "as is": 96.79 %; U = 0.42 %**


The assay "as is" is assessed by quantitative NMR spectroscopy and is equivalent to the assay based on the not-anhydrous and not-dried substance. The assay is verified by titration.

The verified result lies inside our acceptance criteria, i.e. less than 1.0 % difference to assay assigning technique.

For quantitative applications, use the assay as a calculation value on the "as is basis". The uncertainty of the assay can be used for estimation/calculation of measurement uncertainty.

Method 1: Value assigning technique - quantitative NMR spectroscopy	
Conditions	400 MHz, D <sub>2</sub> O
Internal Standard	Potassium hydrogen phthalate (certified reference material), signal 7.2 - 8.1 ppm, 4 H
Result (mass fraction, n = 6)	96.79 %; U = 0.42 %

Quantitative NMR spectrum

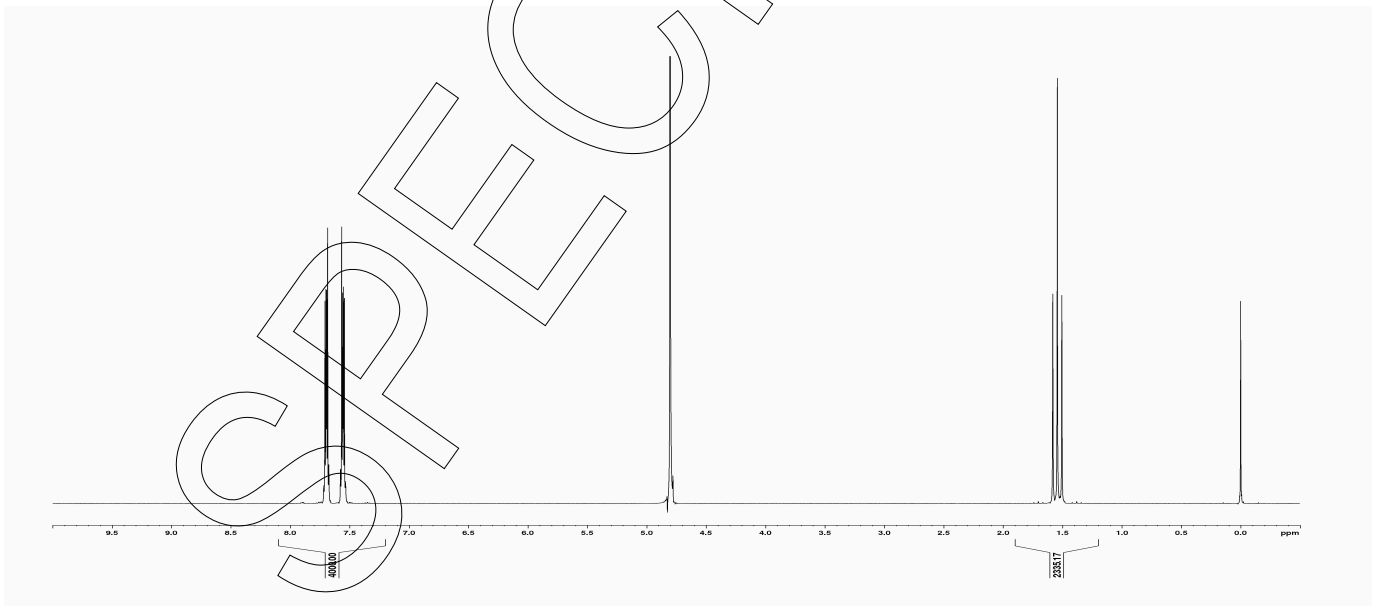



Method 2: Value verifying technique - titration

<b>Conditions</b>	Titration: Mettler Toledo T9 Titrant: 0.1 M HClO <sub>4</sub> Sensor: DGI113-SC
<b>Result</b> (mass fraction, n = 11)	97.35 %

SPECIMEN



## Purity

### Volatile content

#### Water content

<b>Method</b>	Karl Fischer titration
<b>Result</b> (n = 3)	2.77 %*; SD = 0.08 %

\*not accredited testing method

#### Residual solvents

<b>Method</b>	<sup>1</sup> H-NMR
<b>Result</b> (n = 1)	No significant amounts of residual solvents were detected (< 0.05 %).*

\*not accredited testing method

### Inorganic residues

**Method:** Elementary analysis

Inorganic residues can be excluded by elementary analysis (CHN).


SPECIMEN



## Identity

The identity is assessed by ISO/IEC 17025 accredited testing methods.


Method	Conditions	Result
<sup>1</sup> H-NMR	400 MHz, D <sub>2</sub> O	Structure confirmed

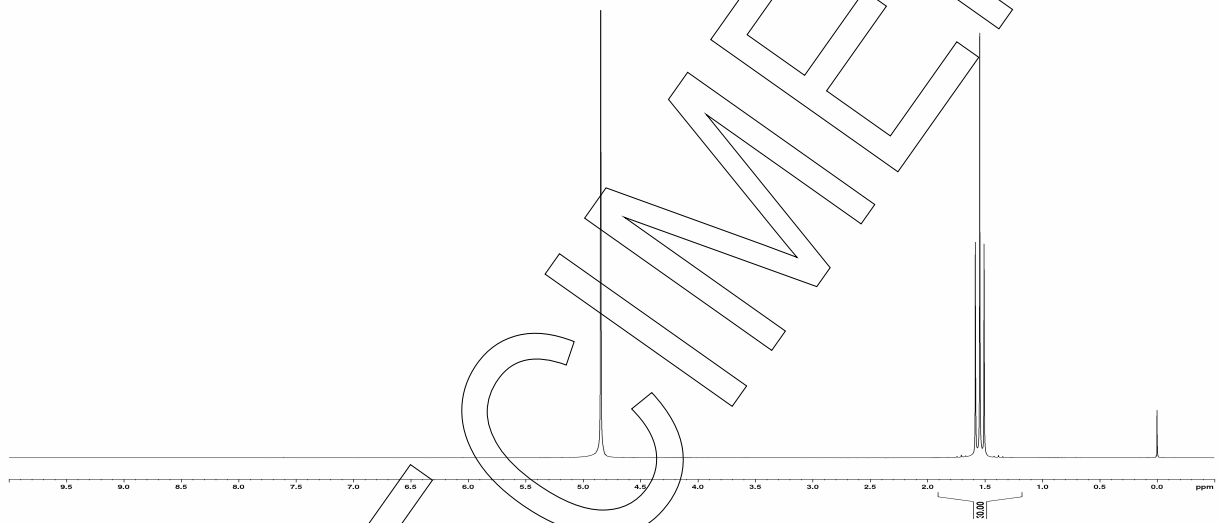



Mikromol™


Method	Conditions	Result
<sup>13</sup> C-NMR	100 MHz, D <sub>2</sub> O	Structure confirmed

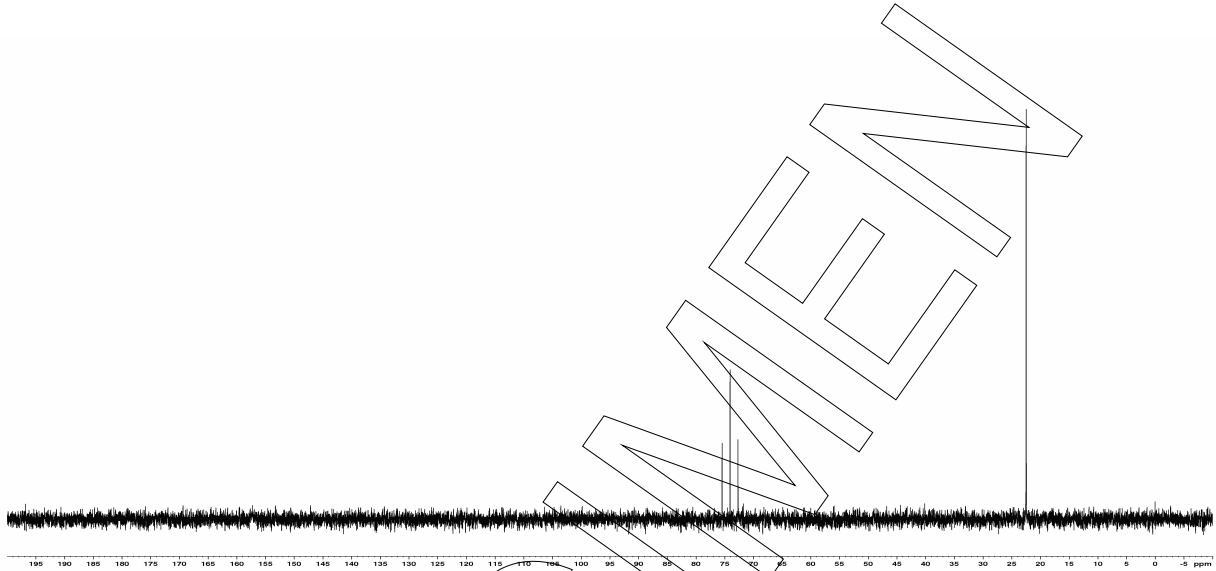



Method	Conditions	Result
MS	3.2 kV ESI-; capillary temperature: 269 °C Theoretical value: 204.96725	Structure confirmed

95203 #1-224 RT: 0.00-1.00 AV: 224 NL: 7.77E7  
T: FTMS - p ESI Full ms [80.00-1000.00]

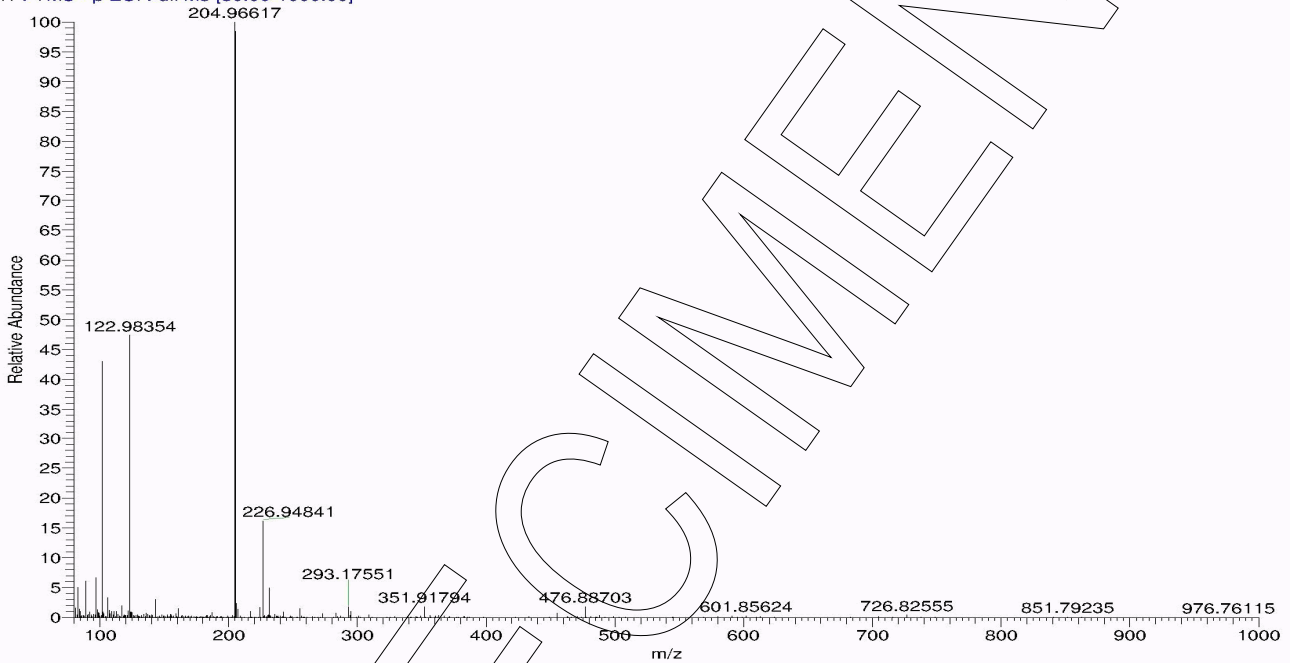


SPECIMEN





Method	Conditions	Result
IR	Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy	Structure confirmed

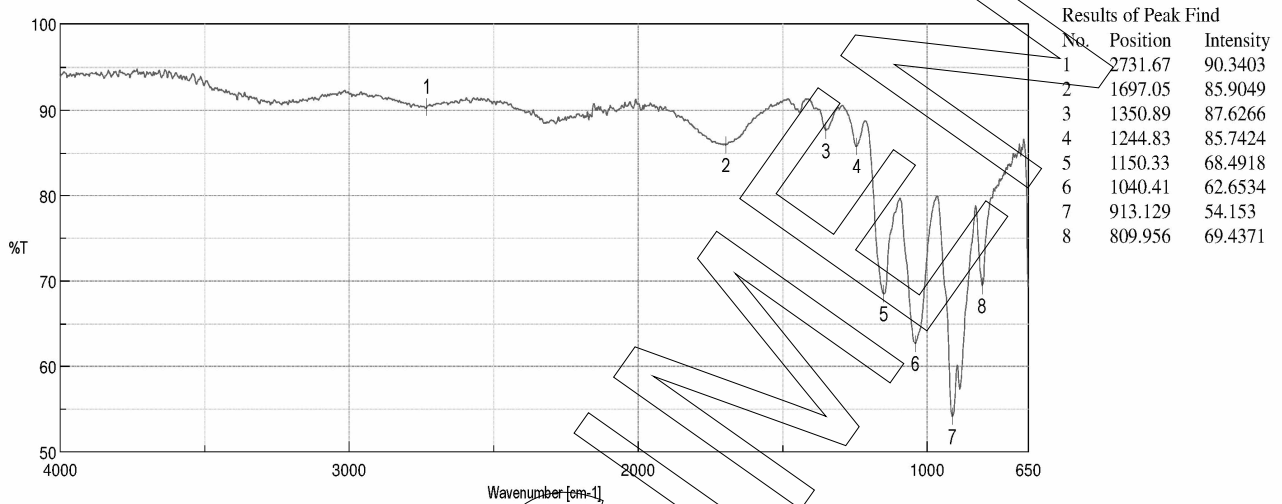

## Stability and Homogeneity

Accelerated stability studies indicate no significant instability. The given validity period is based on this data. This is backed up by additional stability testing and historical data over the range of several years.

RM quality is controlled by regularly performed quality control tests (re tests). Homogeneity assured by qualified process of preparation and verified by homogeneity testing.

## Revision table

Revision	Date	Reason for revision
00	17 Jun 2020	Release of the Certificate of Analysis - initial version

Product warranties for the RM are set out in the terms and conditions of purchase.