

## Certificate of Analysis

## ISO 9001

### Reference Material

#### Product name

2-Ethyl-1,2,3,4-tetrahydro-4,8-isoquinolinediol  
Hydrochloride

#### Product code

MM0035.09-0025

#### CAS number

not listed

#### Molecular weight

229.70

#### Molecular formula

C<sub>11</sub>H<sub>15</sub>NO<sub>2</sub> HCl

#### Lot number

1034885

#### Appearance


white solid

#### Melting point (DSC)

229 °C

#### Long-term storage

2 to 8 °C, dark

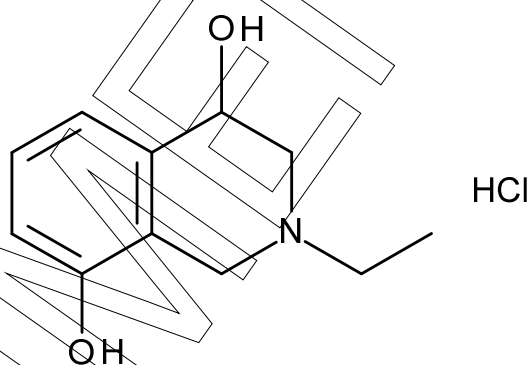

Assay "as is"  
97.5 %

Date of shipment:

**02 Dec 2019**

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **one year** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

<b>Release by:</b>	<b>Date of Release:</b>		Product Release
Dr. Sabine Schröder	Luckenwalde, 08 Oct 2019		



Mikromol™

## Product information

For laboratory use only. Not suitable for human or animal consumption.

Before usage of the RM, it should be allowed to warm to room temperature. No drying required, as the certified value is already corrected for the content of water and other volatile materials.

The product quality is controlled by regularly performed quality control tests (retests).

## Further content

Identity

Assay

Final result

Revision table


SPECIMEN



## Identity


The identity of the reference material was established by following analyses.

Method	Conditions	Result
<sup>1</sup> H-NMR	400 MHz, D <sub>2</sub> O	Structure confirmed

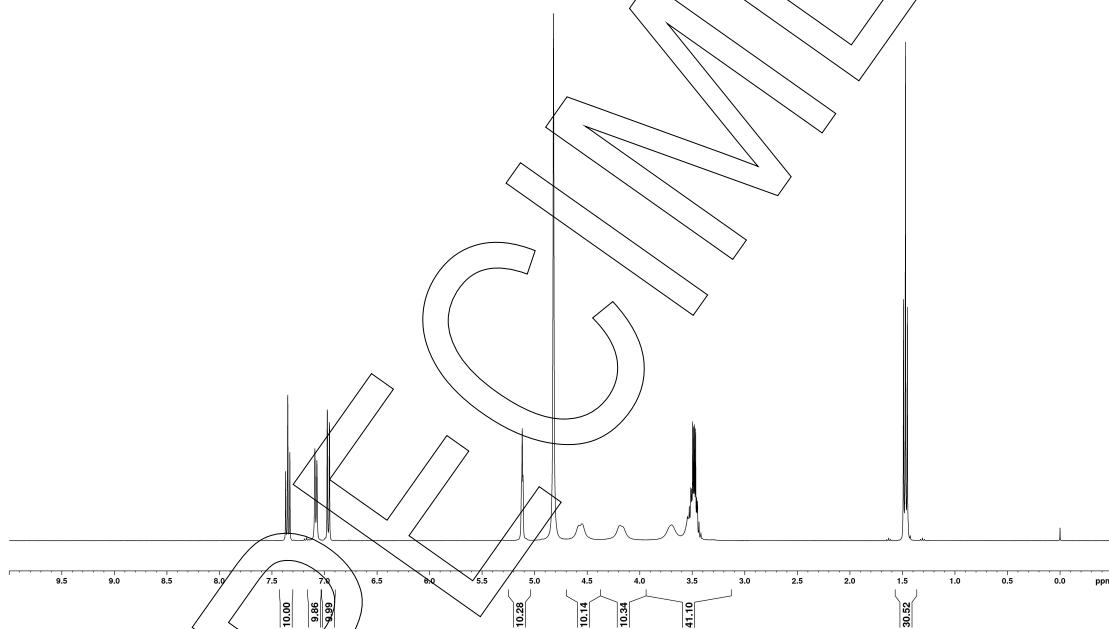




Method	Conditions	Result
MS	3.5 kV ESI+; capillary temperature: 269 °C Theoretical value: 194.11756	Structure confirmed

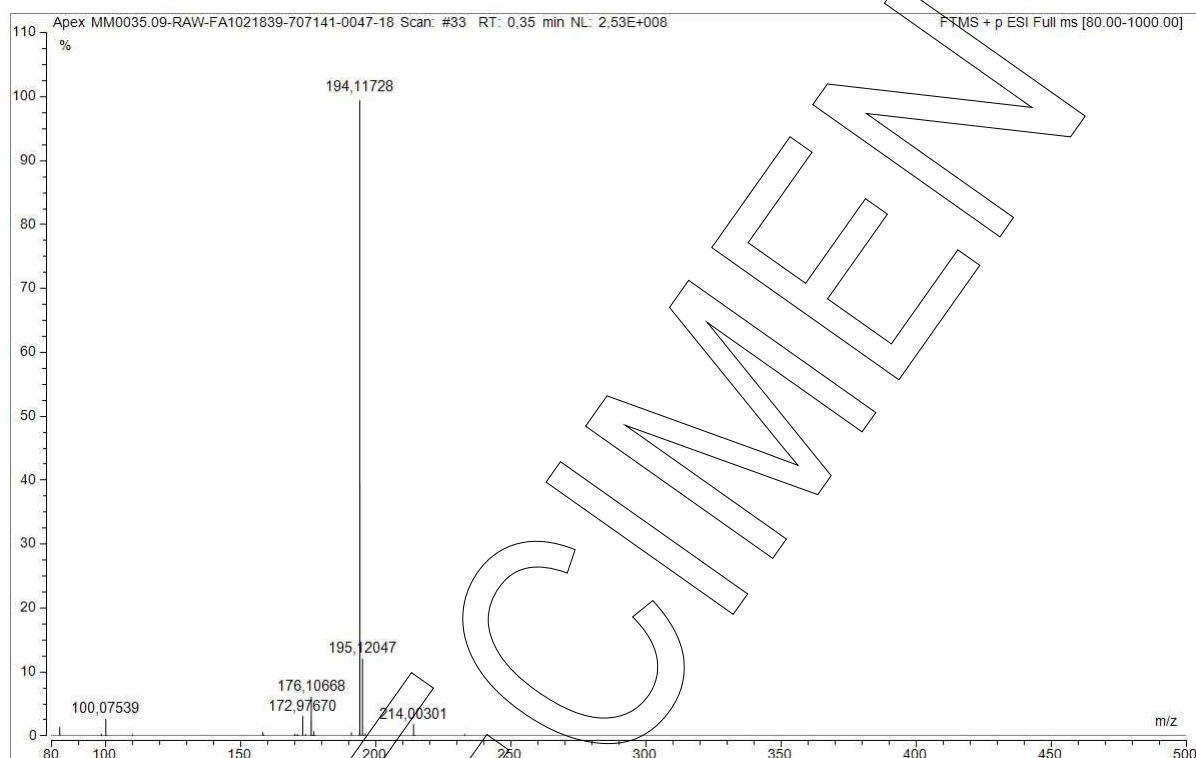



Method	Conditions	Result
IR	Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy	Structure confirmed

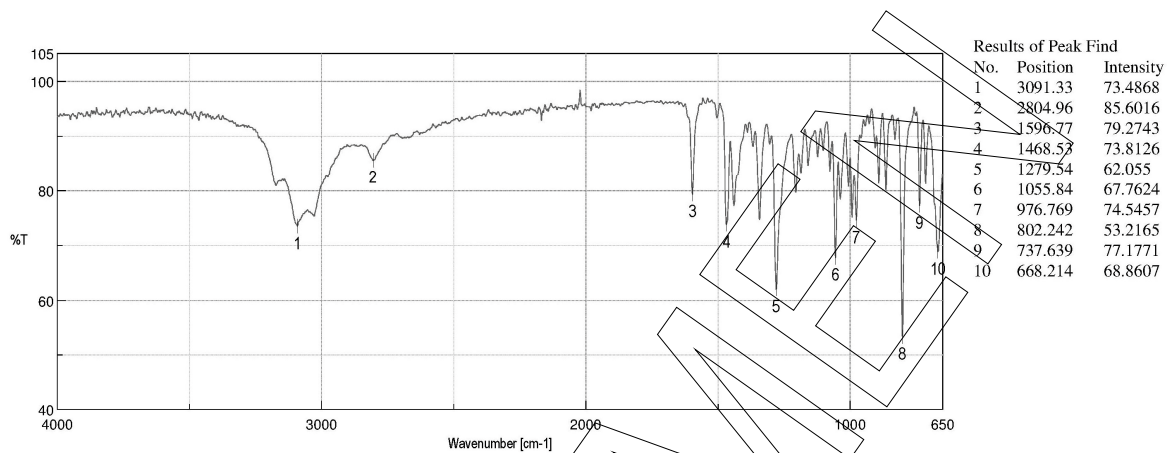




## Assay

The assay of the reference material was assessed by following analyses.

### Purity by High Performance Liquid Chromatography (HPLC)

HPLC conditions:	
Column	Discovery HS F5; 3 µm, 150 x 4.0 mm
Column temperature	40 °C
Detector	DAD, 200 nm
Injector	Auto 2 µl; 0.2108 mg/ml in Water
Flow rate	1.0 ml/min
Phase A	Water, 0.1 % H <sub>3</sub> PO <sub>4</sub>
Phase B	Acetonitrile, 0.1 % H <sub>3</sub> PO <sub>4</sub>
Gradient program	0-10 min A/B 99/1 10-15 min A/B to 60/40 15-20 min A/B 60/40 20-23 min A/B to 99/1 23-35 min A/B 99/1 (v/v)

HPLC chromatogram and peak table

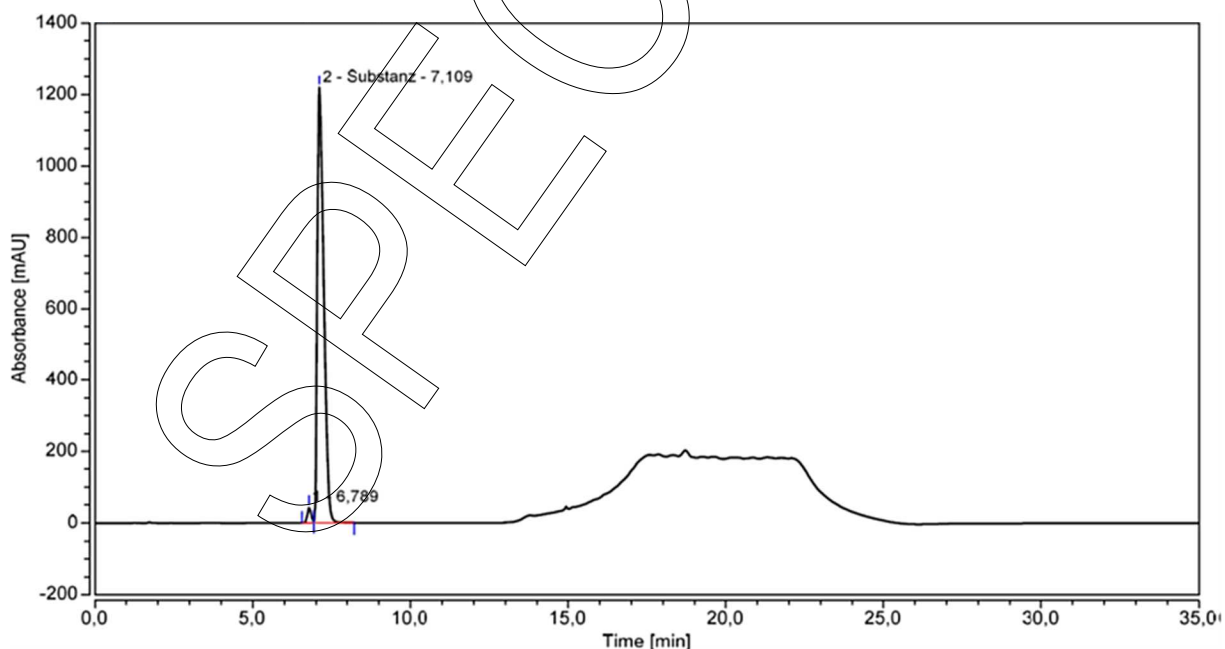



Area percent report - sorted by signal

Pk #	Retention time	Area	Area %
1	6.789	6.065	2.05
2	7.109	289.798	97.95
Totals		295.863	100.00

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

Result (n = 6)

97.97 %; SD = 0.02 %



## Volatile content

Water content	
Method	Karl Fischer titration
Result (n = 3)	0.48 %; SD = 0.03 %

Residual solvents	
Method	<sup>1</sup> H-NMR
Result (n = 1)	No significant amounts of residual solvents were detected (< 0.05 %).

## Final result

**Assay "as is": 97.50 %**

The assay "as is" is assessed by 100% method (mass balance) and is equivalent to the assay based on the not anhydrous and not dried substance respectively.

The calculation of the 100% method follows the formula:

$$\text{Assay (\%)} = (100 \% - \text{volatile contents (\%)}) * \frac{\text{Purity (\%)}}{100 \%}$$

Volatile contents are considered as absolute contributions and purity is considered as relative contribution. Inorganic residues are excluded by additional tests.

## Revision table

Revision	Date	Reason for revision
00	08 Oct 2019	Release of the Certificate of Analysis – initial version

Product warranties for the RM are set out in the terms and conditions of purchase.