



Certificate of Analysis

IARM 63D

Nickel Alloy B-2 / UNS N10665

Certified Reference Material

Certified Values listed in wt.% with associated uncertainties

Al	0.13 ± 0.01	B	0.0017 ± 0.0004	C	0.0079 ± 0.0003	Co	0.013 ± 0.004
Cr	0.153 ± 0.007	Cu	0.003 ± 0.002	Fe	1.56 ± 0.06	Mg	0.0013 ± 0.0007
Mn	0.76 ± 0.02	Mo	26.6 ± 0.1	Nb	0.04 ± 0.01	Ni	70.4 ± 0.2
P	0.004 ± 0.002	S	0.0006 ± 0.0005	Si	0.03 ± 0.02	Ti	0.14 ± 0.01
V	0.007 ± 0.004	W	0.02 ± 0.01	Zr	0.002 ± 0.002		

Indicative Values listed in ppm

Ag (<10)	As (<10)	Au (<1)	Ba (<1)	Be (<1)	Bi (<1)	Br (<1)
Ca (<10)	Cd (<700)	Ce (<1)	Cl (<1)	Cs (<1)	Dy (<1)	Er (<1)
Eu (<1)	F (<1)	Ga (1)	Gd (<1)	Ge (<1)	Hf (<100)	Hg (<1)
Ho (<1)	I (<1)	In (<1)	Ir (<1)	K (<5)	La (<10)	Li (<1)
Lu (<1)	N (7)	Na (<5)	Nd (<8)	O (<60)	Os (<1)	Pb (<10)
Pd (<1)	Pr (<2)	Pt (<1)	Rb (<1)	Re (1)	Rh (<1)	Ru (<1)
Sb (<5)	Sc (<1)	Se (<2)	Sm (<1)	Sn (20)	Sr (<10)	Ta (<110)
Tb (<1)	Te (<3)	Th (<1)	Tl (<1)	Tm (20)	U (<1)	Y (<10)
Yb (<1)	Zn (<3)					

Description and Intended Use

This CRM may come in the form of a solid disc or chips. The intended use of this CRM may include, but is not limited to, the calibration of instruments and the validation of analytical methods.

Interpretation of Data

1. Certified values listed reflect analysis results submitted by qualified analytical laboratories using a combination of methods and instrumentation that emulate actual methods and instrumental techniques currently utilized in the analytical community, and are reported as wt% unless otherwise noted.
2. This material was tested using both the solid disks and chips prepared from individual sections of bar. The certified values are considered representative of the overall average composition of the material.
3. Any data reported and enclosed by a parentheses () is a "best estimate" and is not certified. This data could not be quantified sufficiently for certification. It was, however, reported by enough laboratories to be considered as potentially present in the matrix of the material being examined.
4. "Provisional Certificate of Analysis" reports values that support a fully certified reference material; it also indicates that values may be in a continued process of statistical evaluation and are subject to change.
5. Chips are not certified for Oxygen analysis.



The following data and accompanying statements represent all pertinent information reported in the ILAP as it applies to the chemical characterization of this material.

	Al	B	C	Co	Cr	Cu	Fe	Mg	Mn	Mo	Nb	Ni	P	S	Si	Ti
1	0.10	0.0009	0.007	0.0022	0.13	0.0016	1.43	0.00057	0.69	26.137	0.013	70.0965	0.00061	0.0001	0.00163	0.11
2	0.1	0.0013	0.0078	0.0071	0.14	0.0016	1.515	0.00067	0.756	26.3167	0.017	70.187	0.0010	0.00010	0.0092	0.12
3	0.11	0.0015	0.00793	0.0090	0.147	0.0017	1.52	0.00069	0.76	26.51	0.03	70.31	0.0013	0.0002	0.01	0.1293
4	0.12	0.0016	0.008	0.01	0.15	0.0019	1.5307	0.0008	0.76	26.53	0.033	70.5067	0.003	0.00025	0.013	0.1300
5	0.123	0.00192	0.008	0.01	0.15	0.002	1.55	0.00168	0.76	26.5645	0.0342	70.582	0.004	0.0007	0.021	0.1315
6	0.1275	0.002	0.008	0.0106	0.1500	0.0036	1.5533	0.002	0.766	26.62	0.036	70.65	0.004667	0.0011	0.022	0.132
7	0.13	0.002	0.0081	0.011	0.1519	0.004	1.5614	0.002	0.77	26.6286	0.0380	70.76	0.00475	0.0012	0.0230	0.1363
8	0.134	0.0021	0.0082	0.0118	0.1531	0.0045	1.563		0.771	26.6605	0.05		0.005		0.0232	0.1379
9	0.14	0.0023	0.0083	0.0128	0.16	0.007	1.563		0.7713	26.755	0.055		0.006		0.024	0.14
10	0.14			0.018	0.16		1.62		0.7774	26.79	0.0623		0.0063		0.024	0.14
11	0.1518			0.019	0.161		1.7838		0.7991	26.80					0.03	0.1436
12	0.1541			0.02	0.162										0.0835	0.18
13				0.02667	0.1715										0.0969	
14																
15																
Mean	0.13	0.0017	0.0079	0.013	0.153	0.003	1.56	0.0013	0.76	26.6	0.04	70.4	0.004	0.0006	0.03	0.14
STDV.	0.02	0.0005	0.0004	0.007	0.01	0.002	0.09	0.0007	0.03	0.2	0.02	0.2	0.002	0.0005	0.03	0.02
Certified	0.13	0.0017	0.0079	0.013	0.153	0.003	1.56	0.0013	0.76	26.6	0.04	70.4	0.004	0.0006	0.03	0.14
95% C.I.	0.01	0.0004	0.0003	0.004	0.007	0.002	0.06	0.0007	0.02	0.1	0.01	0.2	0.002	0.0005	0.02	0.01
Methods	X,O,IM,I,G	O,IM,I,G	C	X,O,IM,I,G	X,O,IM,I,G	X,O,IM,I,G	X,O,IM,I,G	O,IM,G	X,O,IM,I,G	X,O,IM,I,G	X,O,IM,I,G	X,O,IM,I,G	X,O,IM,G	X,O,G,C	X,O,IM,I,G	X,O,IM,I,G

	V	W	Zr	Ag	As	Au	Ba	Be	Bi	Br	Ca	Cd	Ce	Cl	Cs	Dy
1	0.00040	0.003	0.00027	0.000078	0.00039	<0.00001	<0.000005	<0.0000005	0.000001	<0.000005	0.000027	<0.00002	<0.000005	0.0000080	<0.00001	<0.000001
2	0.00054	0.0036	0.0005	<0.00005	0.0005	<0.00005	<0.00003	<0.00001	<0.000005	<0.00005	0.000044	<0.00011	<0.00001	<0.000001	<0.00001	<0.000005
3	0.001	0.0040	0.00064	<0.0001	<0.0010	<0.00005	<0.00007	<0.00005	<0.00005		<0.0005	<0.07	<0.00005		<0.00005	<0.00005
4	0.006	0.0047	0.00065	<0.0010	<0.0010				<0.00005		<0.0010					
5	0.0069	0.01	0.0017													
6	0.009	0.018	0.003													
7	0.01	0.0258	0.0037													
8	0.0132	0.026														
9		0.03														
10		0.0372														
11		0.0433														
12																
13																
14																
15																
Mean	0.007	0.02	0.002													
STDV.	0.005	0.01	0.001													
Certified	0.007	0.02	0.002	(<0.001)	(<0.001)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.001)	(<0.07)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.0001)
95% C.I.	0.004	0.01	0.002													
Methods	X,O,IM,G	X,O,IM,G	X,O,IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G

	Er	Eu	F	Ga	Gd	Ge	Hf	Hg	Ho	I	In	Ir	K	La	Li	Lu
1	<0.000001	<0.000001	<0.00001	0.000064	<0.000001	0.000024	0.000009	<0.00001	<0.000001	<0.000001	<0.00001	0.000012	0.000016	<0.000001	<0.000005	<0.000001
2	<0.000005	<0.000005	<0.00001	0.000068	<0.000005	0.000050	0.000012	<0.00005	<0.000005	<0.00001	<0.00001	0.000014	<0.000005	<0.000001	<0.00001	<0.000005
3	<0.00005	<0.00005		0.0001	<0.00005	<0.0001	0.01	<0.00005	<0.00005		<0.00005	<0.00005	<0.0005	<0.00005	<0.00005	<0.00005
4							<0.00005							<0.001		
5							<0.0005							<0.001		
6																
7																
8																
9																
10																
Mean				0.0001			0.01									
STDV.				0.00002			0.007									
Certified	(<0.0001)	(<0.0001)	(<0.0001)	(0.0001)	(<0.0001)	(<0.0001)	(<0.01)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.0005)	(<0.001)	(<0.0001)	(<0.0001)
95% C.I.																
Methods	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	X,IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G

	N	Na	Nd	O	Os	Pb	Pd	Pr	Pt	Rb	Re	Rh	Ru	Sb	Sc	Se
1	0.00045	0.000022	<0.000001	0.0002	0.000014	0.00005	<0.00001	<0.000001	<0.00001	<0.00005	0.0001	<0.00001	<0.00001	0.0001	<0.000005	<0.00005
2	0.0005	<0.000001	<0.000005	0.00024	0.00003	0.000090	<0.00005	<0.000005	<0.00001	<0.0001	0.00012	<0.00001	<0.0001	0.0001	<0.00001	<0.0001
3	0.0007	<0.0005	<0.0008	0.0003	<0.00005	0.0001	<0.00005	<0.0002	<0.00005	<0.0001	0.00012	<0.00005	<0.0001	0.00011	<0.00005	<0.0002
4	0.001			0.006		0.001					<0.0005			<0.0005		
5	<0.0010			<0.0010		<0.0001										
6																
7																
8																
9																
10																
Mean	0.0007			0.002							0.0001					
STDV.	0.0002			0.003							0.00001					
Certified	(0.0007)	(<0.0005)	(<0.0008)	(<0.006)	(<0.0001)	(<0.001)	(<0.0001)	(<0.0002)	(<0.0001)	(<0.0001)	(0.0001)	(<0.0001)	(<0.0001)	(<0.0005)	(<0.0001)	(<0.0002)
95% C.I.																
Methods	F	IM,G	IM,G	F	IM,G	X,O,IM	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G

	Sm	Sn	Sr	Ta	Tb	Te	Th	Tl	Tm	U	Y	Yb	Zn
1	<0.000001	0.00016	<0.00005	0.000029	<0.000001	0.000014	<0.000001	<0.000001	<0.000001	0.0000035	<0.00005	<0.000001	0.000030
2	<0.000005	0.00016	<0.0005	0.000032	<0.000005	<0.00001	<0.000001	<0.000005	<0.000005	0.000007	<0.0001	<0.000005	0.000071
3	<0.00005	0.00020	<0.0010	0.005	<0.00005	<0.0003	<0.00005	<0.00005	<0.00005	<0.00005	<0.0005	<0.00005	<0.0003
4		0.001		0.01089									
5		0.004		<0.00005									
6		0.0045		<0.0005									
7		<0.0005											
8													
9													
10													
Mean		0.002		0.01									
STDV.		0.002		0.005									
Certified	(<0.0001)	(0.002)	(<0.001)	(<0.011)	(<0.0001)	(<0.0003)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.0001)	(<0.001)	(<0.0001)	(<0.0003)
95% C.I.													
Methods	IM,G	X,O,IM,G	IM,G	X,O,IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G	IM,G

Legend: W = Classical, C = Combustion, F = Fusion, A = AA or GFAA, I = ICP or DCP, IM=ICP-MS, D = DC Arc, O = AES, X = XRF, G = GDAES or GDMS, H = Hollow Cathode AES



Participating Laboratories

Anderson Laboratories, Inc. Cannon-Muskegon Laboratorio Prove Materiali S. Marco srl Northern Analytical Laboratory Oxford Instruments Analytical GmbH VHG Labs	Greendale, WI Muskegon, MI Schio, Italy Londonderry, NH Uedem, Germany Manchester, NH	ATI Specialty Materials, Lockport EAG Laboratories Laboratory Testing, Inc. NSL Analytical Services VDM-Metals USA, LLC	Lockport, NY Liverpool, NY Hatfield, PA Cleveland, OH Florham Park, NJ
--	--	---	--

Traceability

Members of the "Inter-Laboratory Analysis Program" (ILAP) validate test methods and instrument performance utilizing SRMs, CRMs, and RMs produced by recognized Certifying Bodies. The specific SRMs, CRMs, and RMs applicable to the material covered by this certificate are:

ALPHA 881	ALPHA AR670	BSH1B	IARM 100B	IARM 274A	IARM 63B	LECO 501-550	LECO 502-016	NIST 343A
ALPHA AR1648	ALPHA AR892	CM 6V3968-3	IARM 202A	IARM 52B	IARM 63C	LECO 501-646	MBH 215XHB1M	NIST 864
ALPHA AR1650	ALPHA AR946	HOCS-001	IARM 203A	IARM 56D	IARM 68C	LECO 501-674	MBH 215XHB5K	NIST 867
ALPHA AR1653	BS CSN-4	HPS-ICV	IARM 241A	IARM 63A	LECO 501-502	LECO 501-991	NIST 1188	NIST 899C
ALPHA AR660	BS H1							

Homogeneity and Uncertainty

"Uncertainty" values, as reported adjacent to certified concentration values, are based on a 95% Confidence Interval. These estimated uncertainties include the combined effects of method imprecision, material inhomogeneity, and any bias between methods. Homogeneity data from experimental XRF results are reflected in both the overall statistics and certified data. Homogeneity samples are selected by a systematic sampling procedure. The number of samples may be determined by equation 1, where N_{prod} is the number of units produced and N_{min} is the number of samples used for homogeneity testing. These samples are arranged in a simple randomized design such that each sample is analyzed multiple times by XRF. Homogeneity is also determined within sample using an applied version of ASTM E826. A single factor ANOVA is used to calculate uncertainty due to inhomogeneity (U_{hom}). Uncertainty of the material is calculated by equation 2, where $H=U_{hom}$, S = Standard deviation, t = t-value at 95% CI, and n = number of observations.

$$1. N_{min} = \max(10, \sqrt[3]{N_{prod}})$$

$$2. U_{CRM} = \frac{\sqrt{H^2 + S^2}}{\sqrt{n}} * t$$

The International Standards Organization (ISO) definitions, expressed in ISO Guide 30-1992 list the following:

Certifying Body: Any technically competent body (organization or firm, public or private) that issues a reference material certificate with the information detailed in ISO Guide 31. The only generally accepted certifying body in the United States for primary standards or Standard Reference Materials (SRM) is the U. S. Department of Commerce, National Institute of Standards & Technology (NIST), Gaithersburg, MD. All other certifying bodies in the United States produce Reference Materials (RM) or Certified Reference Materials (CRM).

Reference Material (RM): Material or substance, with one or more property values that are sufficiently homogeneous and well established, to be used for the calibration of an apparatus, the assessment of a measurement method, or for assigning values to materials.

Certified Reference Material (CRM): Reference material, accompanied by a certificate, with one or more property values certified by a procedure, which establishes its traceability to an accurate realization of the unit in which the property values are expressed, and for which each certified value is accompanied by an uncertainty at a stated level of confidence.


Inter-Laboratory Analysis Program (ILAP): ASTM Standard E691-87 applies to inter-laboratory studies to "Determine the Precision of a Single Test Method", but also outlines a well thought out and logical plan for conducting an inter laboratory program involving multiple analytical techniques. Therefore, the guidelines established in ASTM E691-87 were applied to all aspects of this inter laboratory program, including the protocols for planning, handling, analysis and treatment of resulting data.

Methods of Analysis: The "Inter Laboratory Analysis Program" analyzes a wide variety of materials, and as a result, no single analytical method would provide optimum analytical results. Therefore, a combination of ASTM Standard Methods for classical wet chemistry, ICP, AA, Optical Emission, X-Ray spectrometric, and other accepted methods were used to produce analytical data. Carbon, Sulfur, Nitrogen, and Oxygen results were supplied from combustion and OE instrument procedures.

Expiration of Certification: The certification of this IARM is valid indefinitely, within the uncertainty specified, provided the IARM is handled and stored in accordance with the instructions stated on this certificate. The certification is nullified if the IARM is damaged, contaminated, otherwise modified, or used in a manner for which it was not intended.

Instructions for Use: The test surface is on the side opposite to the labeled surface, which includes the IARM number. The entire thickness of the unit is certified. However, the user is cautioned not to measure disks less than 2 mm thick when using X-ray fluorescence spectrometry. Each packaged disk has been prepared by finishing the test surface using a lathe. The user must determine the correct surface preparation procedure for each analytical technique. The user is cautioned to use care when either resurfacing the disk or performing additional polishing, as these processes may contaminate the surface. The minimum sample size for chips should be individually evaluated based on the analytical technique used; this would typically be greater than 0.1 grams. The material should be stored in a cool, dry location when not in use. **Chips are not to be used for Oxygen analysis.**

Selection of Materials: A "batch" or "series" is defined as a continuous length of bar produced from a single heat. The majority of IARM materials are in wrought condition; other methods of manufacture are utilized if necessary. ILAP samples are removed from equal sections from the total length of the bar. A portion of each section is converted to chips and a thin (pin) disk for analysis by classical wet chemistry, ICP, AA, and combustion procedures, and the balance remains as a thick disk for OES and X-Ray analysis.

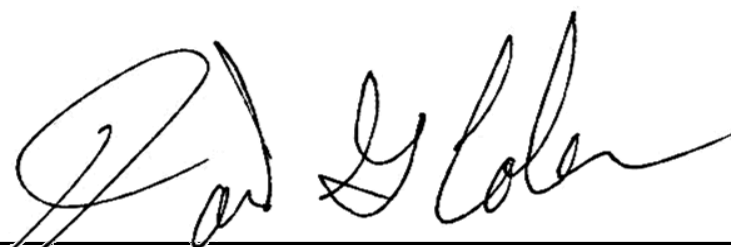

David Coler, General Manager

Analytical Reference Materials International



Analytical Reference Materials International • 276 Abby Road • Manchester, NH 03103
 Telephone (603) 935-4100 • Fax (603) 935-4101 • www.ARMI.com • ARMI@LGCgroup.com

63D-02202018-IARM-F

2/20/2018

3 / 3