

# Gravimetric Certificate

**EHRENSTORFER™**

## Product Identification

20013700 PCB No. 137

Formula C<sub>12</sub>H<sub>4</sub>Cl<sub>6</sub>

Mol.Weight 360.88

CAS No. 35694-06-5

Expiry Date 19.07.2023

Lot Number 201377IO

Store at 20°C in the dark

Please note: The expiry date is valid under recommended storage conditions only.

| Gravimetric Data  |  |                     |          |             |
|---|--|---------------------|----------|-------------|
| Product Name  |  | Conc. (mg/l)        | Purity % | Weight (mg) |
| PCB No. 137   |  | 10.000              | 99.9     | 8.509       |
| Solvent Information   |  |                     |          |             |
| Solvent   | Lot No.  | Exact Quantity (ml) |          |             |
| Iso-Octane  | H355M20  | 850.00              |          |             |
| Traceability Data   |  |                     |          |             |
| 20013700 163610   | neat product   |                     |          |             |
| 20013700 201377IO   | 10.000 mg/l  |                     |          |             |
| Analytical Data   |  |                     |          |             |
| Detection: GC/ECD   | Method Details:  |                     |          |             |
| Column: DB-5, 30 m, ID 0.25 mm  | Injector: 320° C   |                     |          |             |
| Inj.-Vol.: 1.00 µl  | Start Temperature: 120° C for 4 min  |                     |          |             |
| Flow : 1.0 ml/min   | End Temperature: 320° C for 5 min  |                     |          |             |
| Ret.-Time: 15.46 min.   | Gradient: 15° C/min  |                     |          |             |
| Identity check RT   |  |                     |          |             |
| Comment   | Property value was determined by gravimetric measurements and confirmed by peak area comparison. |                     |          |             |
| The uncertainty/tolerance of this standard is +/- 2.0 %, calculated in accordance with the EURACHEM/CITAC Guide - Quantifying Uncertainty in Analytical Measurement - Second Edition. The uncertainty given is the expanded combined uncertainty and represents an estimated standard deviation equal to the positive square root of the total variance of the uncertainty of components. The expanded uncertainty is U w hich is Uc(y)*K, w here K is the coverage factor at the 95% confidence level (K=2). The expanded uncertainty is based on the combination of uncertainties associated w ith each individual operation involved in the preparation of this product. |  |                     |          |             |

Certified on 19.07.2018

by D. Schmid

The Laboratory LGC Labor GmbH is accredited by DAkkS as indicated by the Accreditation Number D-RM-19883-01 & D-PL-19883-01 has shown competence based on ISO Guide 34:2009 with relevant parts of DIN EN ISO/IEC 17025:2005 for production of certified reference materials in form of organic pure substances and in form of single and multi-component solutions organic pure substances.

LGC Labor GmbH · Bgm.-Schlosser-Str. 6 A · 86199 Augsburg · Germany  
Phone +49 821 906080 · Fax +49 821 9060888 · [augsburg.inquiry@lgcgroup.com](mailto:augsburg.inquiry@lgcgroup.com)  
The warranty for this product is limited to the purchasing price of this product.

18.7.18  
m

Data file: 20013700-36-r001.dx

Instrument: ECD

Sample name: 201377IO

Sequence Name: 2018KW28-ECD-0711b


Inj. volume [µl]: 1.0

Injection date: 7/12/2018 9:07:27 AM

Acq. method: PAHK.amx

Location: 80

Sample Description PCB No. 137

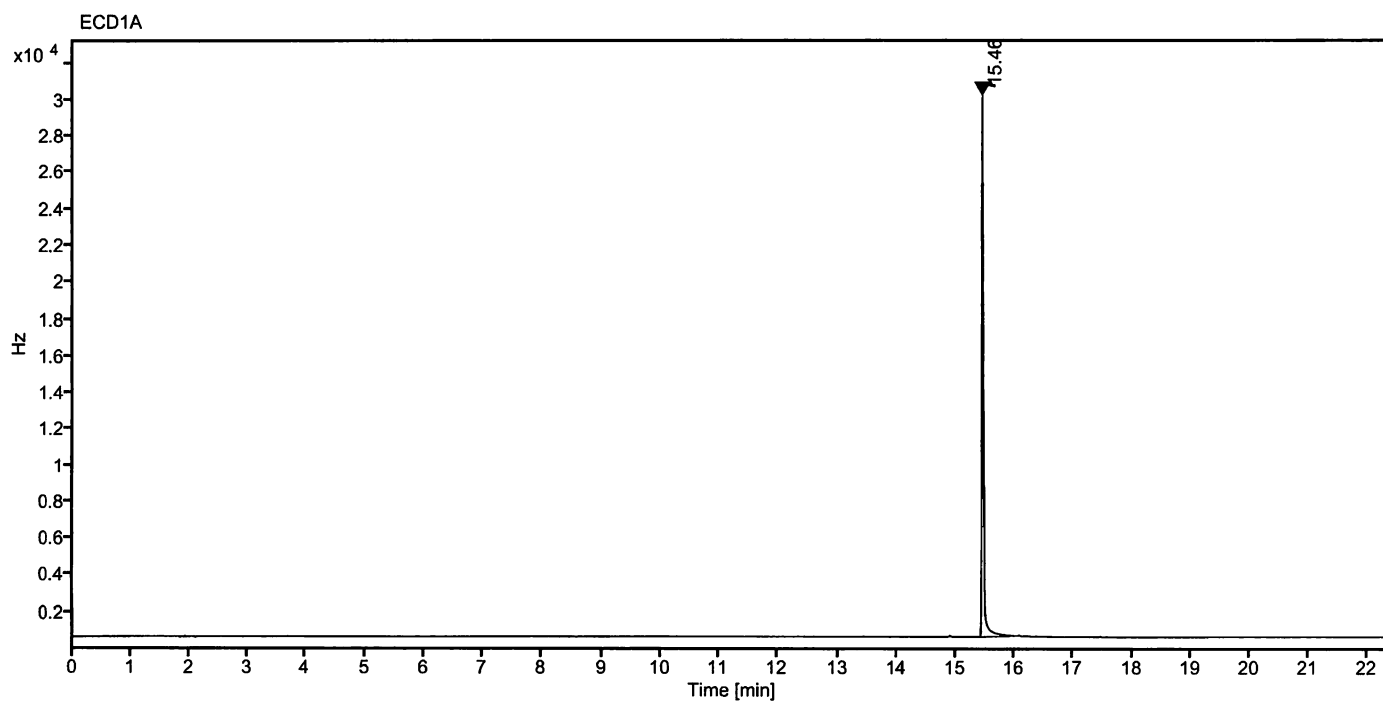

Signal: ECD1A

| Nr. | RT<br>[min] | Area [Hz*s] | Height [Hz] | Area%  | Width<br>[min] |
|-----|-------------|-------------|-------------|--------|----------------|
| 1   | 15.46       | 57672.11115 | 29578.00    | 100.00 | 0.029          |
| Sum |             | 57672.11    |             |        |                |

Schmid D