


Certified Reference Material - Certificate of Analysis

Salicylic Acid-D₄, Primary Standard

Cerilliant Quality
ISO GUIDE 34
ISO/IEC 17025
ISO 13485
ISO 9001
GMP/GLP

Catalog Number: S-042
Lot: FN03211402
Retest: May 2018
Description: Salicylic Acid-D₄ in Acetonitrile
Packaging: Solution in 2 mL amber USP Type I glass ampoule containing not less than 1 mL of certified solution.
Storage: Store unopened in freezer (-10 °C to -25 °C).
Shipping: Ambient. See Stability Section.
Intended Use: This Certified Reference Material is suitable for *their vitro* identification, calibration, and quantification of the analyte(s) in analytical and R&D applications. Not suitable for human or animal consumption.
Instructions for Use: Users should quantitatively transfer desired volume using established good laboratory practices to spike into matrix or to dilute to the desired concentration. Each ampoule is intended for one-time use.
Safety: **Danger. See Safety Data Sheet**



- Retest Date - stability studies ongoing. Certificate of Analysis will be updated upon completion of retest.
- Ampoules are overfilled to ensure a minimum 1 mL volume can be transferred when using a 1 mL Class A volumetric pipette.
- For MS Applications, we advise laboratories not to mix lots during a single sequence.

Analyte	Certified Concentration Value
Salicylic Acid-D ₄	100.0 ± 0.5 µg/mL
<ul style="list-style-type: none"> Uncertainty of the concentration is expressed as an expanded uncertainty in accordance with ISO 17025 and Guide 34 at the approximate 95% confidence interval using a coverage factor of $k = 2$ and has been calculated by statistical analysis of our production system and incorporates uncertainty of the mass balance purity factor, material density, balance, and weighing technique. This standard is prepared gravimetrically and mass results are reported on the conventional basis for weighing in air. Nominal concentration is calculated based on: the actual measured mass; Mass Balance Purity Factor of the analyte(s); measured mass of the solution; and the density of the pure diluent at 20 °C. Concentration is corrected for chromatographic purity, residual water, residual solvents and residual inorganics. No adjustment required before use. Additional certification information available upon request. 	

Metrological Traceability

- This standard has been prepared and certified under the ISO Guide 34, ISO/IEC 17025, ISO 9001 and ISO 13485 standards. This standard meets the requirements of a Certified Reference Material and a Primary Standard as defined by ISO and is traceable to the SI and higher order standards through an unbroken chain of comparisons.
- This standard has been gravimetrically prepared using balances that have been fully qualified and calibrated to ISO 17025 requirements. All calibrations utilize NIST traceable weights which are calibrated externally by a qualified ISO 17025 accredited calibration laboratory to NIST standards. Qualification of each balance includes the assignment of a minimum weighing by a qualified and ISO 17025 accredited calibration vendor taking into consideration the balance and installed environmental conditions to ensure compliance with USP tolerances of NMT 0.1% relative error. Balance calibration adjustments are performed weekly utilizing the balance's internal adjustment mechanism. Calibration verifications are performed pre-use. Weigh tapes from the calibration verification are included in the production batch record for this standard. Production data package available upon request.
- Fill volume is gravimetrically verified throughout the dispensing process using qualified and calibrated balances.
- Concentration is verified against an independently prepared calibration solution gravimetrically prepared.
- Each raw material utilized has been identified and thoroughly characterized through the use of multiple analytical techniques. Spectral data is provided on subsequent pages of this COA. The density and material Mass Balance Purity Factor is traceable to the SI and higher order reference standards through mass measurement and instrument qualification and calibrations.

Cerilliant certifies that this standard meets the specifications stated in this certificate and warrants this product to meet the stated acceptance criteria through the expiration/retest date when stored unopened as recommended. Product should be used shortly after opening to avoid concentration changes due to evaporation. Warranty does not apply to ampoules stored after opening.




Darron Ellsworth, Quality Assurance Manager

May 7, 2014

Date

Solution Standard Verification

Concentration accuracy and within- and between-bottle homogeneity are analytically verified against an independently prepared calibration solution and to the prior lot.

Solution standard verification demonstrates confirmation that the specified requirements for the Primary Standard have been fulfilled and validated under ISO 13485.

Standard Solution Assay Parameters				Calibration Curve	
Analysis Method:	UV/Vis			Calibration Curve:	Linear Regression
Wavelength:	230 nm			Number of Points:	4
Slit Width:	1.0 nm			Linearity (r):	1.000
Response:	0.5 s				

Standard Solution	Lot Number	Verified Concentration (µg/mL)		%RSD - Homogeneity	
		Actual Results	Acceptance Criteria	Actual Results	Acceptance Criteria
New Lot	FN03211402	100.1	± 3%	0.2	≤ 3%
Previous Lot	FN080411-03	99.0	± 3%		

- Concentration is verified through multiple analyses and is calculated as the average of multiple analyses compared to an independently prepared calibration solution.
- Within-sample and between-sample homogeneity of the New Lot is ensured through rigorous production process controls statistically analyzed to evaluate risk and verified by analysis. Multiple samples pulled from across the lot using a random stratified sampling plan were analyzed to verify homogeneity. % RSD results shown above for the New Lot demonstrate ampoule-to-ampoule homogeneity.

Analyte Certification - Mass Balance Purity Factor

Each analyte is thoroughly identified and characterized using an orthogonal approach. A mass balance purity factor is assigned incorporating chromatographic purity and residual impurities. The mass balance purity factor is utilized to calculate the weighing adjustment necessary to ensure accuracy of the solution standard concentration.

Material Name:	Salicylic Acid-D ₄	Chemical Formula:	C ₇ H ₂ D ₄ O ₃
Material Lot:	PN070711-03	CAS Number:	78646-17-0
		Molecular Weight:	142.15


Material Characterization Summary			
Analytical Test	Method	Results	
Primary Chromatographic Purity by HPLC/UV Analysis	SP10-0102	99.9%	
Secondary Purity Analysis by Thin Layer Chromatography	SP10-0106	Single Spot, R _f = 0.38	
Identity by LC/MS Analysis	SP10-0107	Consistent with Structure	
Isotopic Purity by LC/MS SIM Analysis	SP10-0107	0.00% D ₀ vs D ₄	
		0.00% D ₀ to D ₁	7.27% D ₃
		0.22% D ₂	92.51% D ₄
Identity by ¹ H-NMR Analysis	USP <761>, SP10-0116	Consistent with Structure	
Residual Solvent Analysis by GC/FID Headspace	AM1087 ¹	None Detected	
Residual Water Analysis by Karl Fischer Coulometry	USP <921>, SP10-0103	0.01%	
Inorganic Content by Microash Analysis	SP10-0135	< 0.2%	
Purity Factor		99.94%	

- The primary chromatographic purity is calculated as the average of two independently performed analyses utilizing two different methods. Acceptance criteria requires the purity values to be within 0.5% of each other.
- The primary chromatographic purity value is used to calculate the Mass Balance Purity Factor.
- A secondary chromatographic purity method is utilized as a control.
- Mass Balance Purity Factor = [(100 - wt% residual solvent - wt% residual water - wt% residual inorganics) x Chromatographic Purity/100].
- Mass Balance Purity Factor does not include adjustment for chiral and/or isotopic purity.

¹ Validated analytical method

Spectral and Physical Data

HPLC/UV

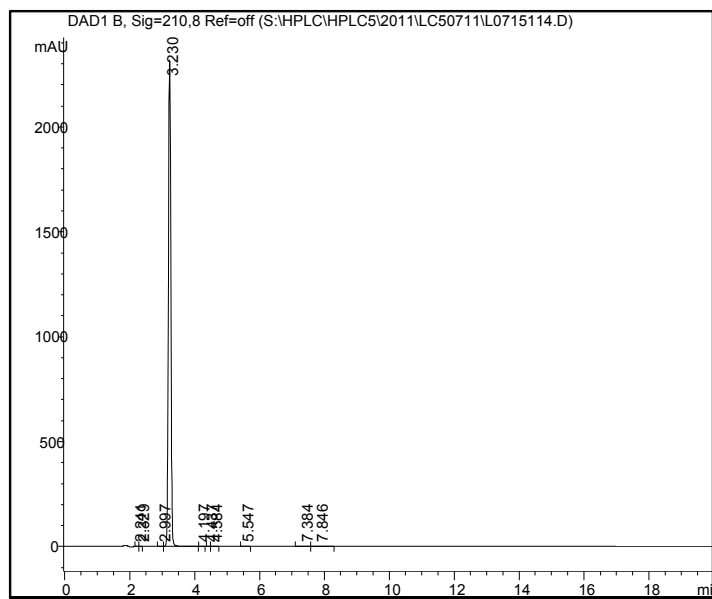


Column: Hypersil Gold Phenyl 5 μ , 4.6 x 150 mm
Mobile Phase: Acetonitrile::0.1% H₃PO₄ (40::60)
Flow Rate: 1.0 mL/min
Wavelength: 210 nm

Data File Name: S:\HPLC\HPLC5\2011\LC50711\L0715114.D
Instrument: LC#5
Sample Name: PN070711-03
Acquired: July 15, 2011

Peak #	Ret Time	Area	Height	Area %
1	2.24	1.12	0.33	0.01
2	2.33	0.73	0.22	0.01
3	3.00	1.02	0.15	0.01
4	3.23	12544.20	2318.75	99.90
5	4.20	0.46	0.10	0.00
6	4.44	0.40	0.08	0.00
7	4.58	1.34	0.21	0.01
8	5.55	0.96	0.14	0.01
9	7.38	1.90	0.17	0.02
10	7.85	4.09	0.34	0.03


¹H NMR

Instrument: JEOL ECS 400
Solvent: DMSO-D₆

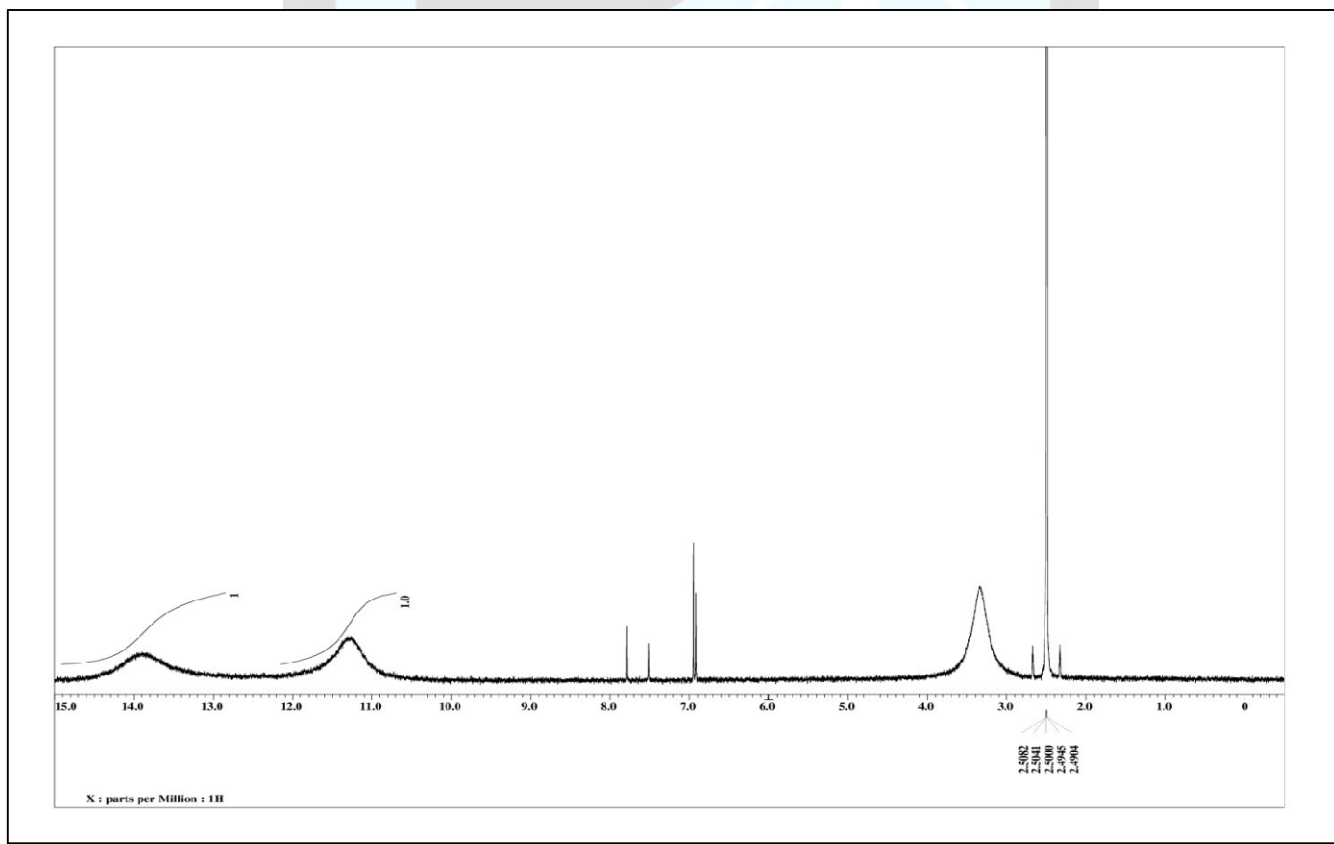

Spectral and Physical Data (cont.)

Residual Solvent Analysis by GC/FID Headspace

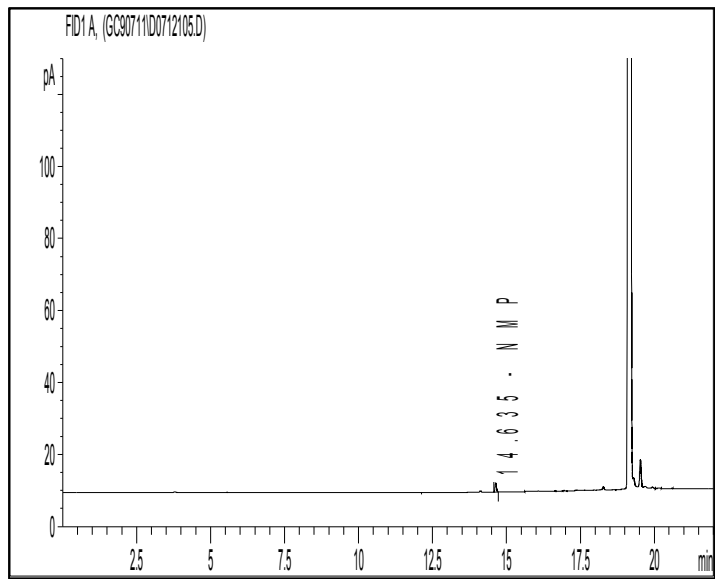

Column: DB-ALC1 30 m x 0.53 mm, 3 µm film thickness
Temp Program: 40°C (12 min) to 220°C at 40°C/min (5.5 min)
Carrier Gas: Helium
Flow Rate: 2.0 mL/min
Detector Heater Temp: 250°C
Injector: Headspace Sampler
HS Oven Temp: 60°C
Vial Equilibration: 10 minutes

Data File Name: C:\CHEM32\1\DATA\GC90711\D0712105.D
Instrument: GC#9
Sample Name: PN070711-03
Acquired: July 12, 2011

Peak	Compound	Area	Weight %
1	NMP	NA	NA
Total			ND


ND - Not Detected

Spectral and Physical Data (cont.)

LC/MS

Column: Zorbax Eclipse RRHD 1.8 μ C₁₈, 2.1 x 50 mm
Mobile Phase: 0.1% Formic acid in Water::0.1% Formic acid in Acetonitrile (70::30)
Flow Rate: 0.4 mL/min
Scan Range: 50-1200 amu

Ionization: Electrospray, Negative Ion
Data File Name: W07141133
Instrument: Waters XEVO G2 QTOF
Sample Name: PN070711-03
Acquired: July 14, 2011

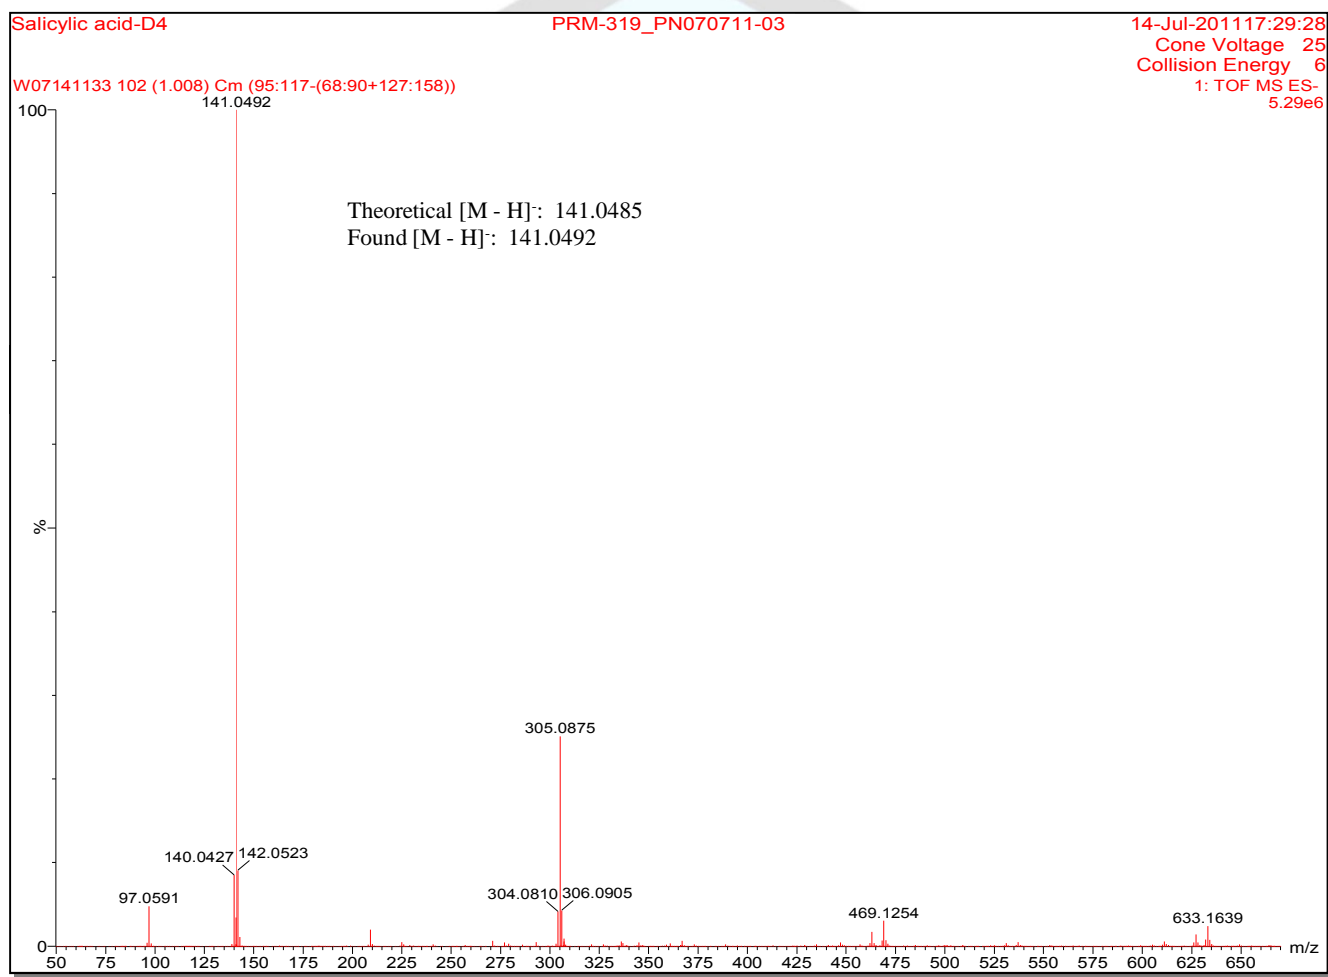


Spectral and Physical Data (cont.)

Isotopic Purity by LC/MS SIM Analysis

Column: Zorbax Eclipse RRHD 1.8 μ C₁₈, 2.1 x 50 mm
Mobile Phase: 0.1% Formic acid in Water::0.1% Formic acid in Acetonitrile (70::30)
Flow Rate: 0.4 mL/min
Scan Range: 137-141 amu

Ionization: Electrospray, Negative Ion
Data File Name: W07141133
Instrument: Waters XEVO G2 QTOF
Sample Name: PN070711-03
Acquired: July 14, 2011 5:29 PM

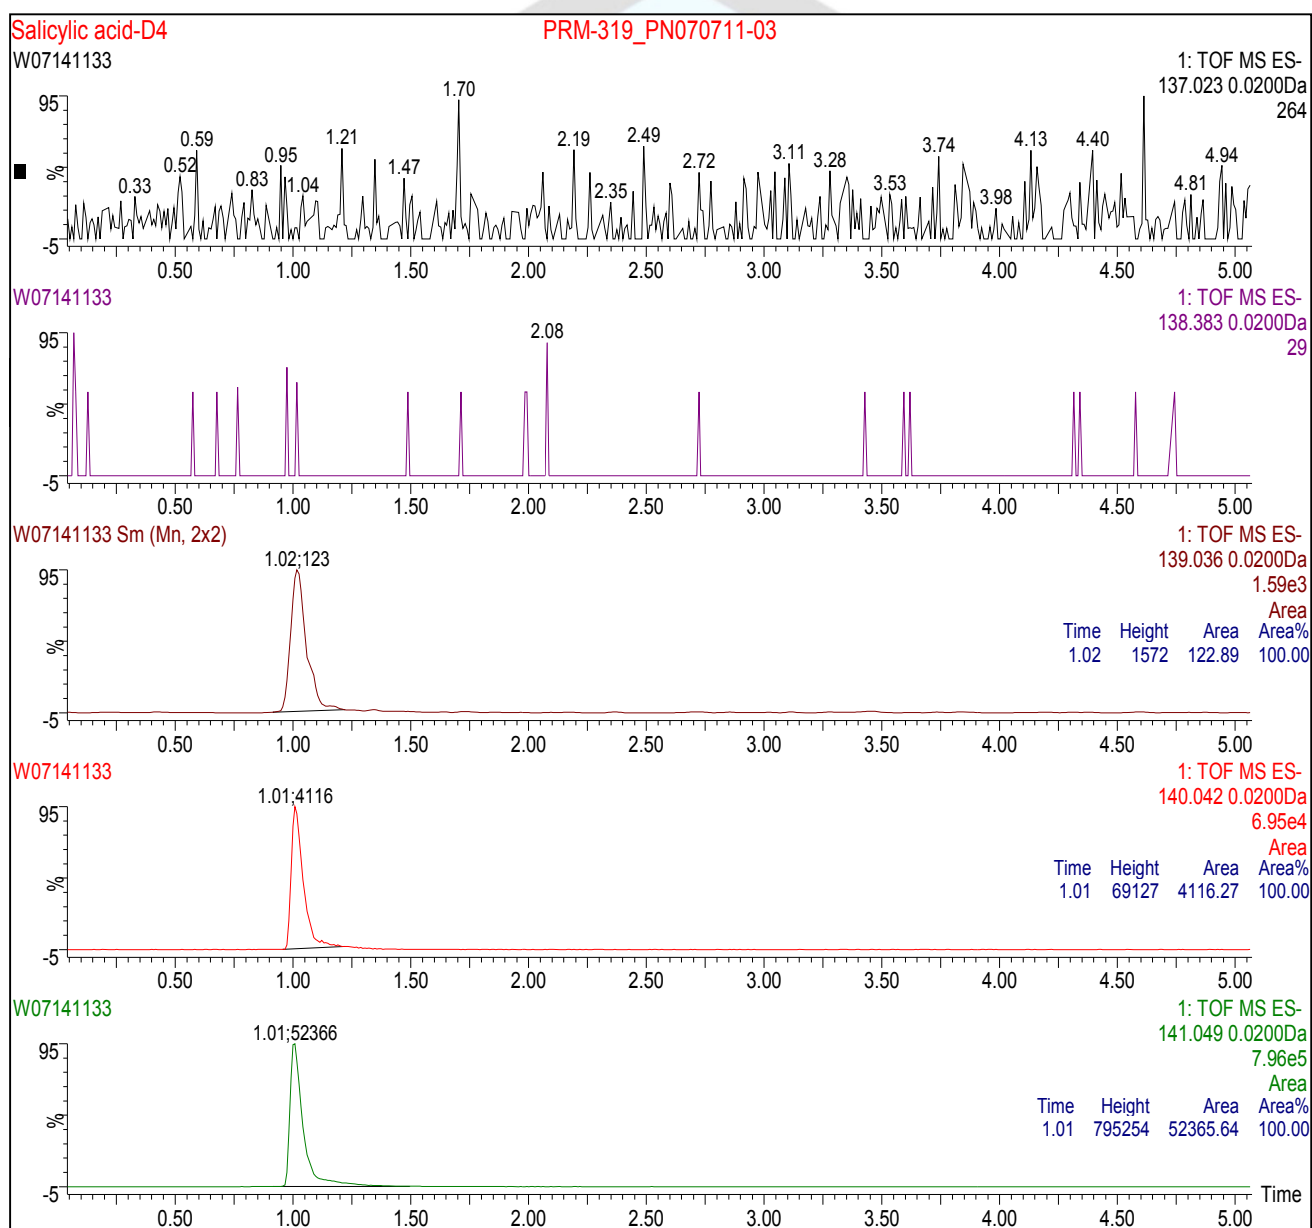

Stability

Short term stability studies have been performed under accelerated conditions for a period of up to four weeks. Short term data is utilized to predict long term stability and to support transport conditions and normal laboratory use. Real-time stability studies are performed at the recommended storage conditions over the life of the product.

Short Term Stability : A summary of accelerated stability findings for this product is listed below.		
Storage Condition	Mean Kinetic Temperature (MKT)	Time Period/Result
Freezer	-15°C	No decrease in purity was noted after four weeks.
Refrigerator	4°C	
Room Temperature	21°C	
40°C	40°C	
Transport/Shipping : Stability data supports transport of this product at ambient conditions.		
Short Term Storage: Stability data supports short term storage up to 3 months at Refrigerate conditions.		
Long Term Stability: Long term stability has been assessed for Freezer storage (-10 °C to -25 °C) conditions. Stability of a minimum of 35 months has been established through real-time stability studies.		

COA Revision History

Revision No.	Date	Reason for Revision
00	May 7, 2014	Initial version