



## Certificate of Analysis

## ISO 17034

### Reference Material

#### Product name

Quinine Dihydrochloride

#### Product code

MM0458.00

#### CAS number

60-93-5

#### Molecular weight

397.34

#### Molecular formula

C<sub>20</sub>H<sub>24</sub>N<sub>2</sub>O<sub>2</sub> · 2HCl

#### Lot number

G1062698

#### Appearance


white solid

#### Melting point (DSC)

226 °C

#### Long-term storage

2 to 8 °C, dark

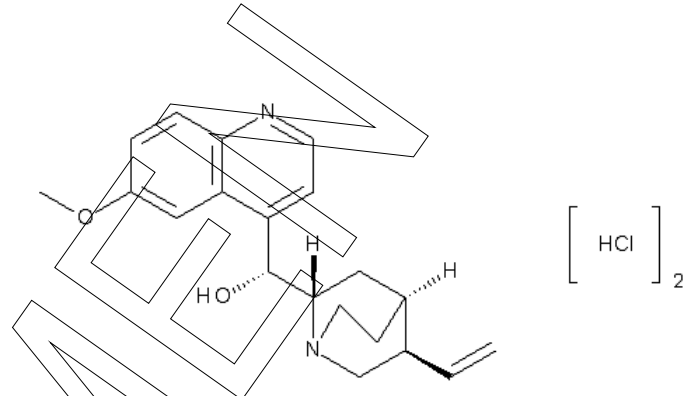

Assay<sup>1</sup> "as is"  
**94.3 %**

Uncertainty<sup>2</sup> U  
**0.4 %**

**Intended Use:** Use for identification and quantification. The assay is verified by a second testing method. Due to the homogeneity studies, the minimum amount of sample to be used is 10 mg.

Date of shipment: **02 Feb 2021**

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **two years** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

<b>Release by:</b>	<b>Date of Release:</b>		Product Release
Dr. Sabine Schröder	Luckenwalde, 03 Jul 2020		

<sup>1</sup> Calibration and verification were carried out using standards traceable to SI-units. The value is expressed on an "as is" basis.

<sup>2</sup> The uncertainty "U" is the expanded uncertainty of the testing method for the assigned value estimated in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM). It corresponds to a level of confidence of about 95%. Coverage factor k = 2.



## Important product information

This RM is intended for laboratory use only and is not suitable for human or animal consumption.

This RM conforms to the characteristics of a primary standard as described in the ICH Guidelines. The values quoted in this Certificate of Analysis are the producer's best estimate of the true values within the stated uncertainties and based on the techniques described in this Certificate of Analysis. The production of this RM was undertaken in accordance with the requirements of ISO 17034. The identity is verified by data from international scientific literature.

## Storage and handling

Before usage of the RM, it should be allowed to warm to room temperature. No drying is required, as assigned values are already corrected for the content of water and other volatile materials.

## Further content

Assigned value

Purity

Identity

Stability and homogeneity

Revision table

SPECIMEN



## Assigned value

**Assay "as is": 94.31 %; U = 0.35 %**

The assay "as is" is assessed by 100% method (mass balance) and is equivalent to the assay based on the not-anhydrous and not-dried substance. The assay is verified by quantitative NMR spectroscopy. The verified result lies inside our acceptance criteria, i.e. less than 1.0 % difference to assay assigning technique.

For quantitative applications, use the assay as a calculation value on the "as is basis". The uncertainty of the assay can be used for estimation/calculation of measurement uncertainty.

### Method 1: Value assigning technique - 100% method

**100% method (mass balance) with chromatographic purity by HPLC**

**Result**

94.31 %; U = 0.35 %

The calculation of the 100% method follows the formula:

$$\text{Assay (\%)} = (100\% - \text{volatile contents (\%)}) * \frac{\text{Purity (\%)}}{100\%}$$


Volatile contents are considered as absolute contributions and purity is considered as relative contribution. Inorganic residues are excluded by additional tests.



Method 2: Value verifying technique - quantitative NMR spectroscopy

Conditions	400 MHz, DMSO-d <sub>6</sub> / D <sub>2</sub> O
Internal Standard	1,2,4,5-Tetramethylbenzene (certified reference material), signal 6.8 - 7.0 ppm, 2 H
Result (mass fraction, n = 6)	94.68 %

Quantitative NMR spectrum

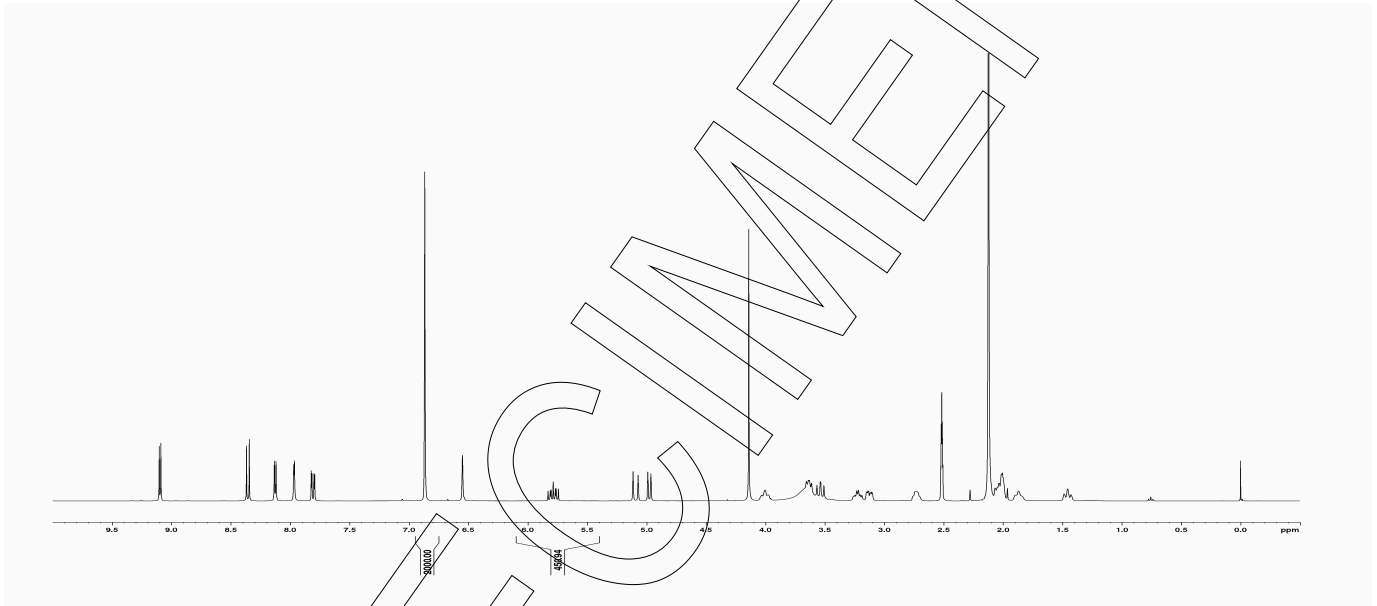




## Purity

### Purity by high performance chromatography (HPLC)

HPLC Conditions:	
Column	BetaBasic 8; 5 $\mu\text{m}$ , 100 x 4.6 mm
Column temperature	40 °C
Detector	DAD, 250 nm
Injector	Auto 2 $\mu\text{l}$ , 0.1014 mg/ml in Acetonitrile/Water 50/50 (v/v)
Flow rate	1.0 ml/min
Phase A	Water, 0.1 % $\text{H}_3\text{PO}_4$
Phase B	Acetonitrile, 0.1 % $\text{H}_3\text{PO}_4$
Gradient program	0-10 min A/B 90/10 10-15 min A/B to 50/50 15-20 min A/B 50/50 20-23 min A/B to 90/10 23-30 min A/B 90/10 (v/v)

### HPLC chromatogram and peak table

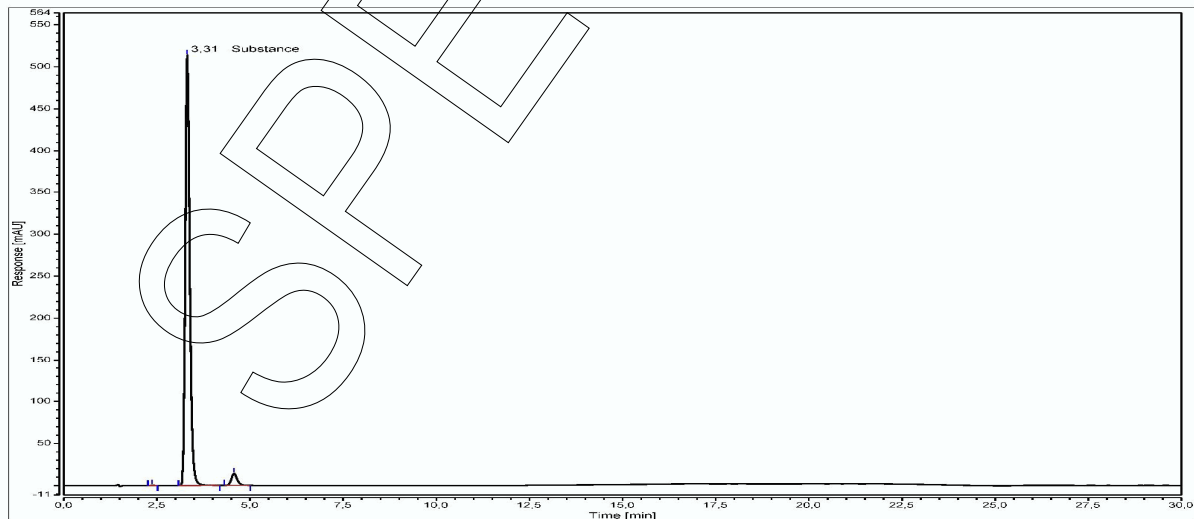



## Area percent report - sorted by signal

Pk #	Retention time	Area	Area %
1	2.371	0.0352	0.05
2	3.311	71.9931	96.55
3	4.571	2.5351	3.40
<b>Totals</b>		<b>74.5634</b>	<b>100.00</b>

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

**Result (n = 10)** 96.52 %; U = 0.33 %

## Volatile content

### Water content

**Method** Karl Fischer titration  
**Result (n = 3)** 2.29 %\*; SD = 0.02 %

\*not accredited testing method

### Residual solvents

**Method** GC headspace  
**Result (n = 3)** No significant amounts of residual solvents were detected (< 0.05 %).

## Inorganic residues

**Method:** Sulphated ash, EP-8.2 chapter 2.4.14


According to the available data, the presence of inorganic impurities in the reference material other than those detectable by sulphated ash is highly unlikely. Inorganic residues can be excluded by results of the sulphated ash. Therefore, no assay correction was performed for inorganic impurities.



## Identity


The identity is assessed by ISO/IEC 17025 accredited testing methods.

Method	Conditions	Result
<sup>1</sup> H-NMR	400 MHz, DMSO-d <sub>6</sub>	Structure confirmed

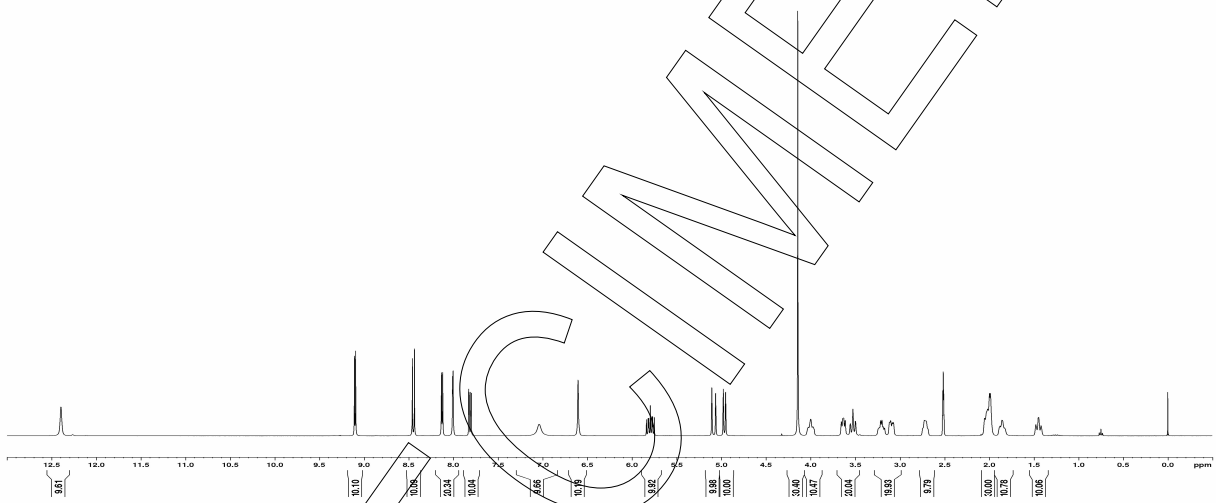



Method	Conditions	Result
<sup>13</sup> C-NMR	100 MHz, DMSO-d <sub>6</sub>	Structure confirmed

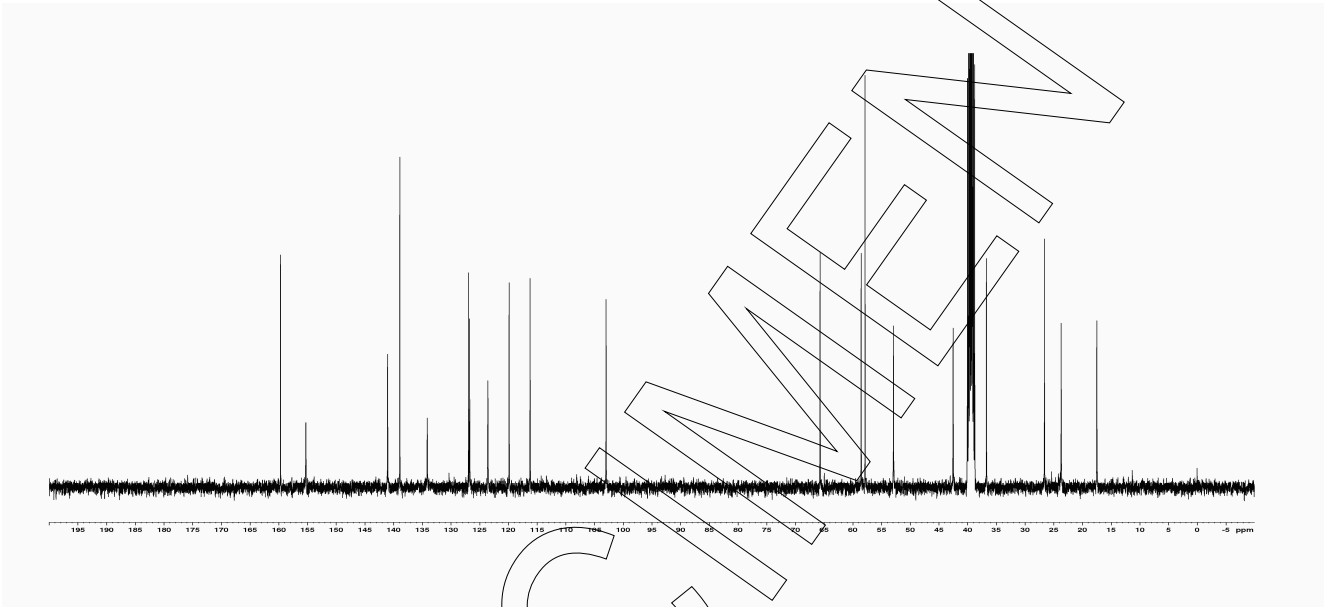


SPECIMEN






Method	Conditions	Result
MS	3.5 kV ESI+; capillary temperature: 269 °C Theoretical value: 325.19105	Structure confirmed

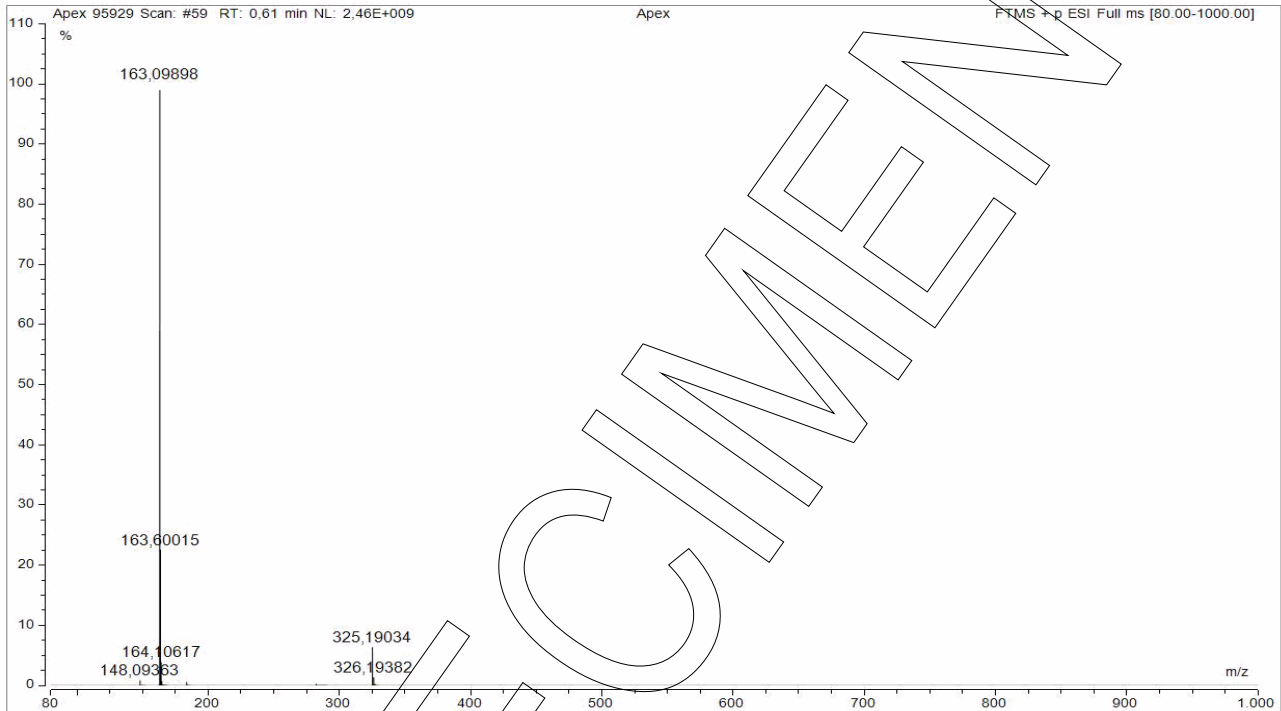



Method	Conditions	Result
IR	Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy	Structure confirmed

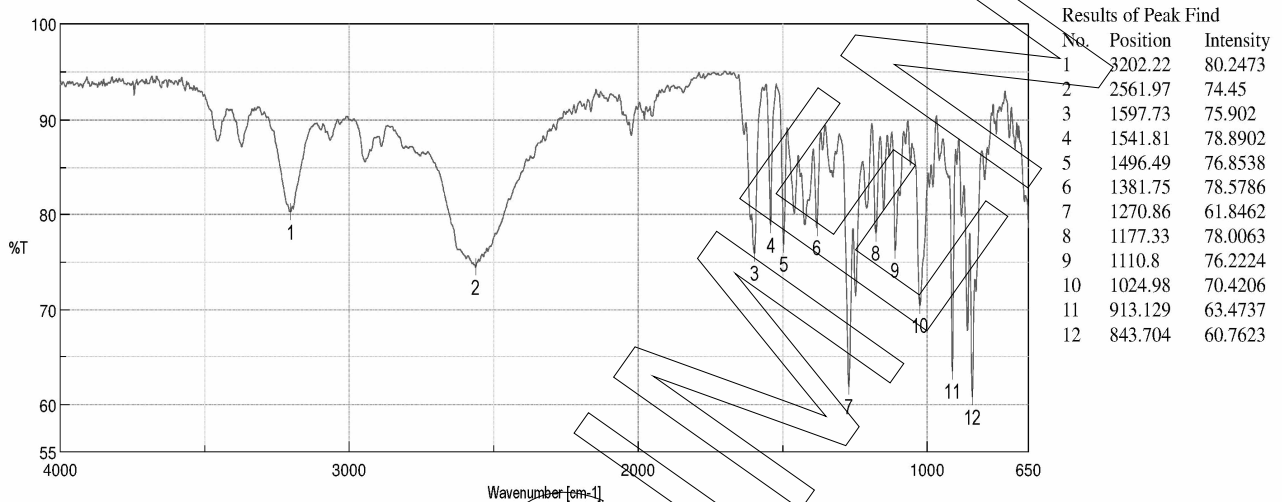

Method	Conditions	Result
Optical Rotation	c = 2.0 in 0.1 M HCl	$[\alpha]_D^{20} = -219^\circ$

## Stability and Homogeneity

Accelerated stability studies indicate no significant instability. The given validity period is based on this data. This is backed up by additional stability testing and historical data over the range of several years.

RM quality is controlled by regularly performed quality control tests (re tests). Homogeneity assured by qualified process of preparation and verified by homogeneity testing.



### Revision table

Revision	Date	Reason for revision
00	08 Jul 2020	Release of the Certificate of Analysis - initial version

Product warranties for the RM are set out in the terms and conditions of purchase.

SPECIMEN