

Certificate of Analysis

ISO 17034

Reference Material

Product name

Fenbendazole

Product code

MM0518.00-0250

CAS number

43210-67-9

Molecular weight

299.35

Molecular formula

C₁₅H₁₃N₃O₂S

Lot number

G1017550

Appearance


off-white solid

Melting point

231 °C

Long-term storage

2 to 8 °C, dark

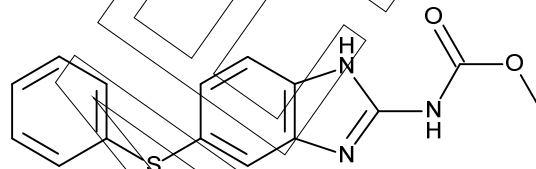

Assay¹ "as is"
99.95 %

Uncertainty² U
0.4 %

Intended Use: Use for identification and quantification. The assay is verified by a second testing method. Due to the homogeneity studies, the minimum amount of sample to be used is 10 mg.

Date of shipment: **02 Feb 2021**

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **two years** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

Release by:	Date of Release:		Product Release
Dr. Sabine Schröder	Luckenwalde, 27 Jan 2021		

¹ Calibration and verification were carried out using standards traceable to SI-units. The value is expressed on an "as is" basis.

² The uncertainty "U" is the expanded uncertainty of the testing method for the assigned value estimated in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM). It corresponds to a level of confidence of about 95%. Coverage factor k = 2.



Important product information

This RM is intended for laboratory use only and is not suitable for human or animal consumption.

This RM conforms to the characteristics of a primary standard as described in the ICH Guidelines. The values quoted in this Certificate of Analysis are the producer's best estimate of the true values within the stated uncertainties and based on the techniques described in this Certificate of Analysis. The production of this RM was undertaken in accordance with the requirements of ISO 17034. The identity is verified by data from international scientific literature.

Storage and handling

Before usage of the RM, it should be allowed to warm to room temperature. No drying is required, as assigned values are already corrected for the content of water and other volatile materials.

Further content

Assigned value

Purity

Identity

Stability and homogeneity

Revision table

SPECIMEN



Assigned value


Assay "as is": **99.95 %; U = 0.41 %**

The assay "as is" is assessed by quantitative NMR spectroscopy and is equivalent to the assay based on the not-anhydrous and not-dried substance. The assay is verified by 100% method (mass balance). The verified result lies inside our acceptance criteria, i.e. less than 1.0 % difference to assay assigning technique.

For quantitative applications, use the assay as a calculation value on the "as is basis". The uncertainty of the assay can be used for estimation/calculation of measurement uncertainty.

Method 1: Value assigning technique - quantitative NMR spectroscopy	
Conditions	400 MHz, DMSO-d ₆
Internal standard	Maleic acid (certified reference material), signal 5.9 – 6.6 ppm, 2 H
Result (mass fraction, n = 6)	99.95 %, U = 0.41 %

Quantitative NMR spectrum

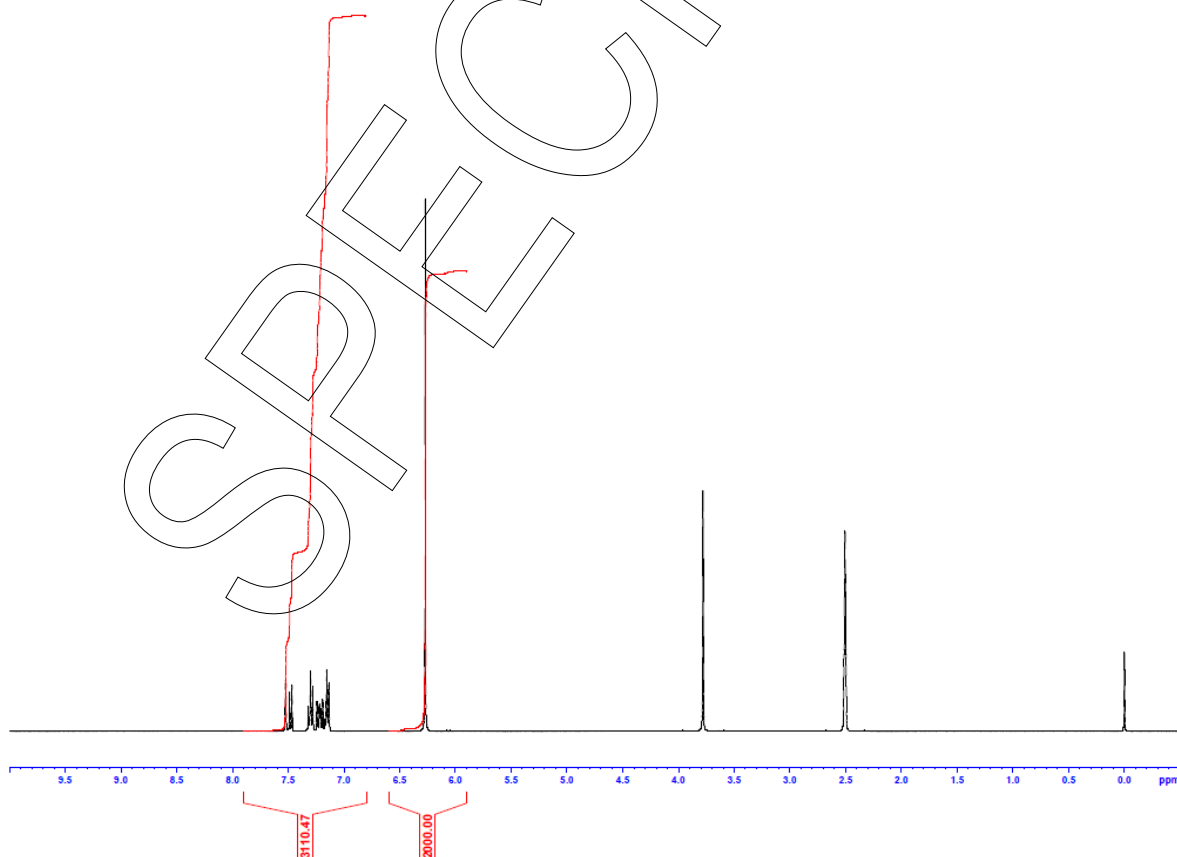



Method 2: Value verifying technique - 100% method

100% method (mass balance) with chromatographic purity by HPLC

Result

99.81 %

The calculation of the 100% method follows the formula:

$$\text{Assay (\%)} = (100 \% - \text{volatile contents (\%)}) * \frac{\text{Purity (\%)}}{100 \%}$$

Volatile contents are considered as absolute contributions and purity is considered as relative contribution. Inorganic residues are excluded by additional tests.

Purity

Purity by High Performance Liquid Chromatography (HPLC)

HPLC conditions:

Column

Hypersil Gold C18; 5 µm, 150 x 4.6 mm

Column temperature

40 °C

Detector

DAD, 280 nm

Injector

Auto 4 µl; 0.162 mg/ml in Acetonitrile; 0.1 % H₃PO₄

Flow rate

1.0 ml/min

Phase A

Water, 0.1 % H₃PO₄

Phase B


Acetonitrile, 0.1 % H₃PO₄

Gradient program

0-8 min A/B 70/30
8-11 min A/B to 40/60
11-13 min A/B to 70/30
13-20 min A/B 40/60 (v/v)



HPLC chromatogram and peak table

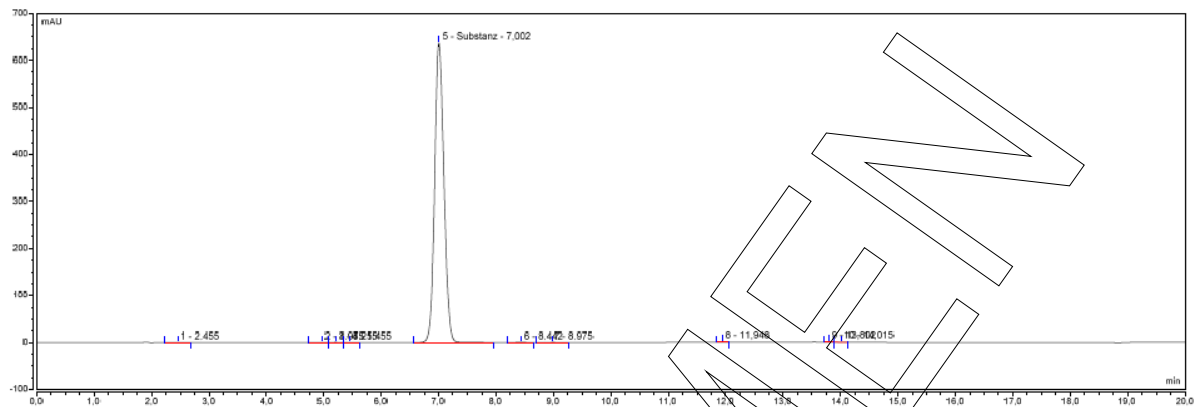

Area percent report - sorted by signal

Pk #	Retention time	Area	Area %
1	2.455	0.0256	0.02
2	4.975	0.0221	0.02
3	5.215	0.0220	0.02
4	5.455	0.0155	0.01
5	7.002	119.1366	99.81
6	8.442	0.0306	0.03
7	8.975	0.0321	0.03
8	11.948	0.0508	0.04
9	13.802	0.0083	0.01
10	14.015	0.0189	0.02
Totals		119.3626	100.00

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

Result (n = 6)

99.81 %; U = 0.19 %



Volatile content

Loss on drying	
Method	105 °C for 4 h, EP 10.3, chapter 2.2.32
Result (n = 3)	No significant amounts of volatile contents were detected (< 0.05 %).

Inorganic residues

Method: Sulphated ash, EP 10.3, chapter 2.4.14

According to the available data, the presence of inorganic impurities in the reference material other than those detectable by sulphated ash is highly unlikely. Inorganic residues can be excluded by results of the sulphated ash. Therefore, no assay correction was performed for inorganic impurities.


SPECIMEN



Identity


The identity is assessed by ISO/IEC 17025 accredited testing methods.

Method	Conditions	Result
¹ H-NMR	400 MHz, DMSO-d ₆	Structure confirmed

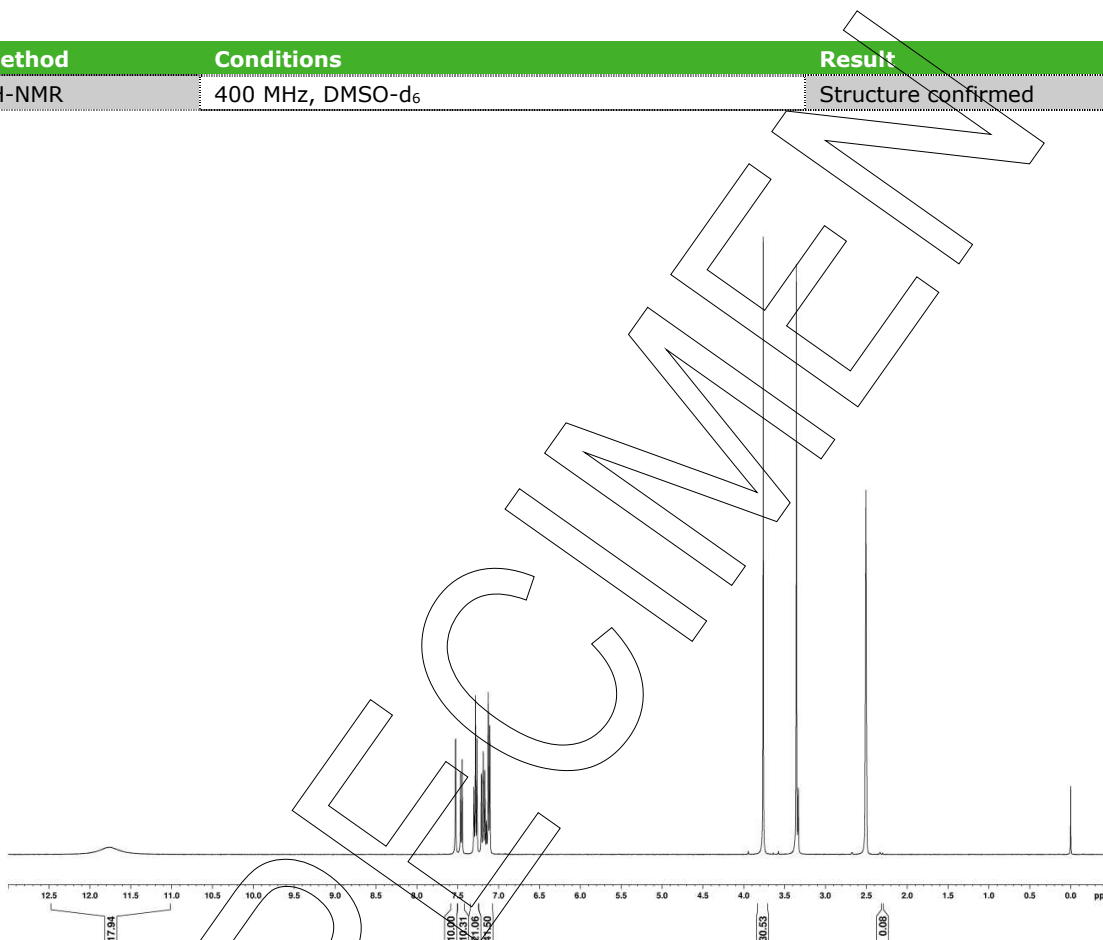




Method	Conditions	Result
MS	4.5 kV ESI+; vaporization temperature: 200 °C	Structure confirmed

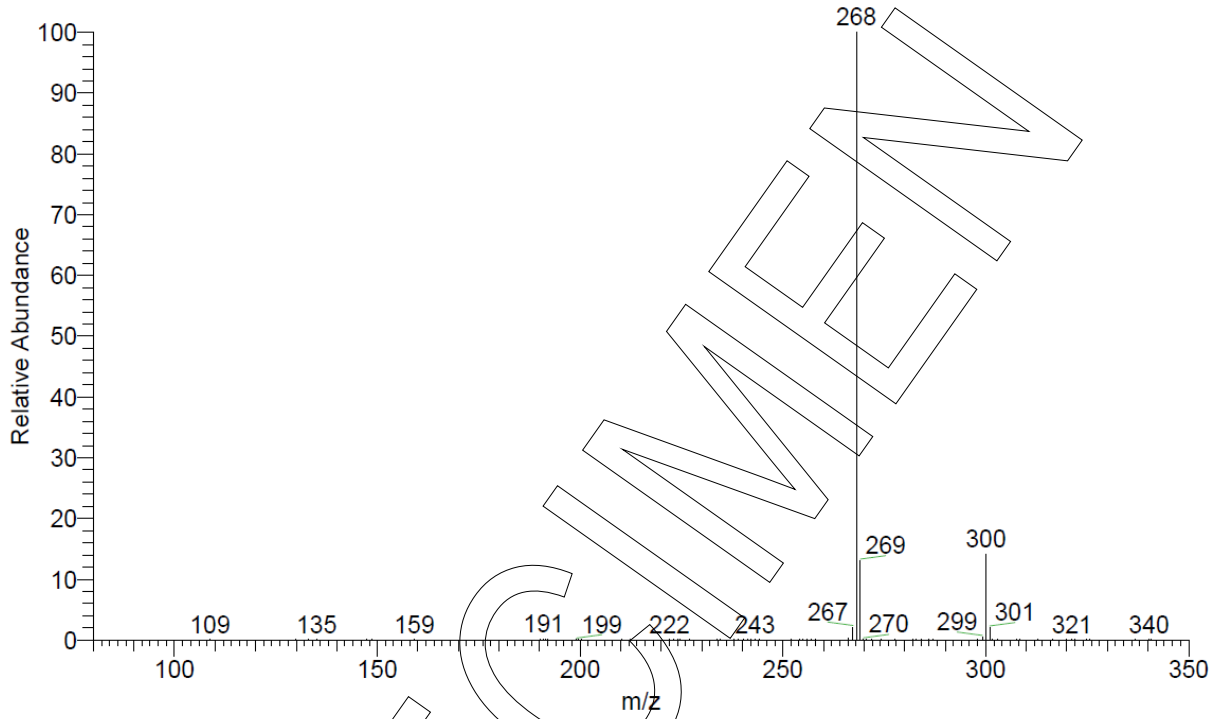



Method	Conditions	Result
IR	Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy	Structure confirmed

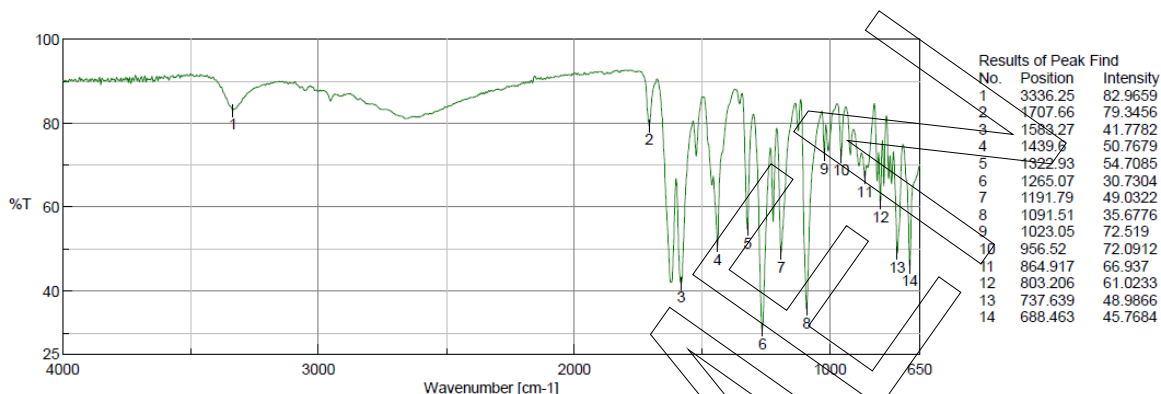

Stability and homogeneity

The assessment of stability indicates no significant instability. The given validity period is based on this data. This is backed up by additional stability testing and historical data over the range of several years.

RM quality is controlled by regularly performed quality control tests (re tests). Homogeneity assured by qualified process of preparation and verified by homogeneity testing.

Revision table

Revision	Date	Reason for revision
00	27 Jan 2021	Release of the Certificate of Analysis - initial version

Product warranties for the RM are set out in the terms and conditions of purchase.