



## Certificate of Analysis

### Reference Material

#### Product name

7-Chloro-1-cyclopropyl-4-oxo-6-(piperazin-1-yl)-1,4-dihydroquinoline-3-carboxylic Acid

#### Product code

MM0018.02

#### CAS number

133210-96-5

#### Molecular weight

347.80

#### Molecular formula

C<sub>17</sub>H<sub>18</sub>ClN<sub>3</sub>O<sub>3</sub>

#### Lot number

1018966

#### Appearance


beige solid

#### Melting point

251 °C (dec)

#### Long-term storage

2 to 8 °C, dark  
hygroscopic

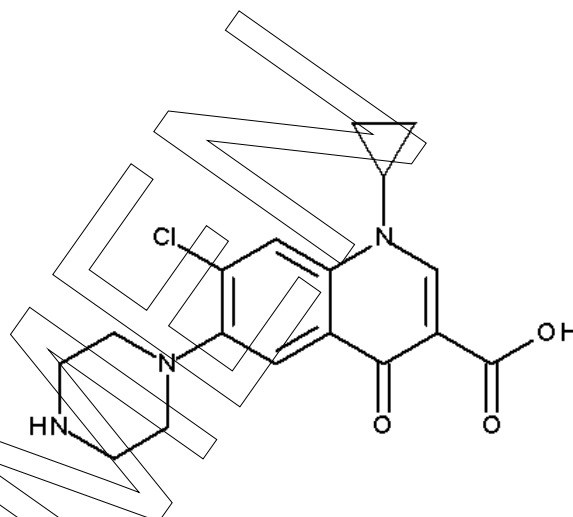

Assay "as is"  
91.4 %

Date of shipment:

**15 Jul 2022**

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **two years** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

<b>Release by:</b>	<b>Date of Release:</b>		Product Release
Dr. Sabine Schröder	Luckenwalde, 02 Oct 2019		



**Mikromol<sup>TM</sup>**

## Product information

For laboratory use only. Not suitable for human or animal consumption.

Before usage of the RM, it should be allowed to warm to room temperature. No drying required, as the certified value is already corrected for the content of water and other volatile materials.

The product quality is controlled by regularly performed quality control tests (retests).

## Further content

Identity

Assay

Final result


Revision table

SPECIMEN

## Identity


The identity of the reference material was established by following analyses.

Method	Conditions	Result
<sup>1</sup> H-NMR	400 MHz, CF <sub>3</sub> COOD	Structure confirmed

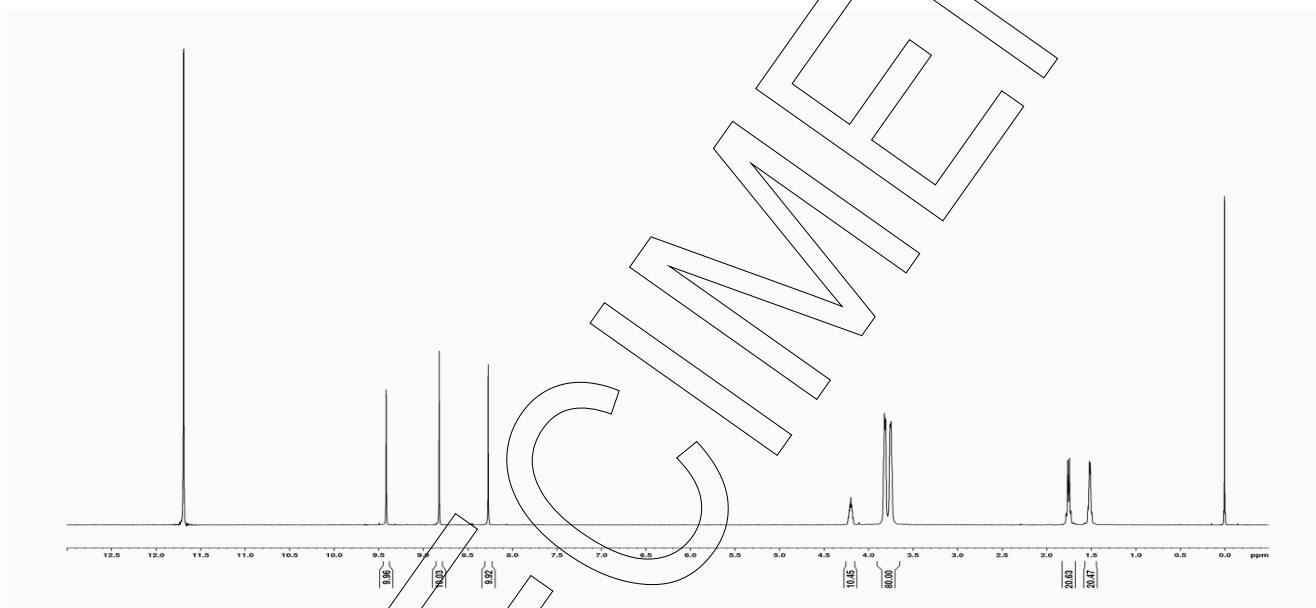




Method	Conditions	Result
MS	3.5 kV ESI+; capillary temperature: 269 °C Theoretical value: 348.11095	Structure confirmed

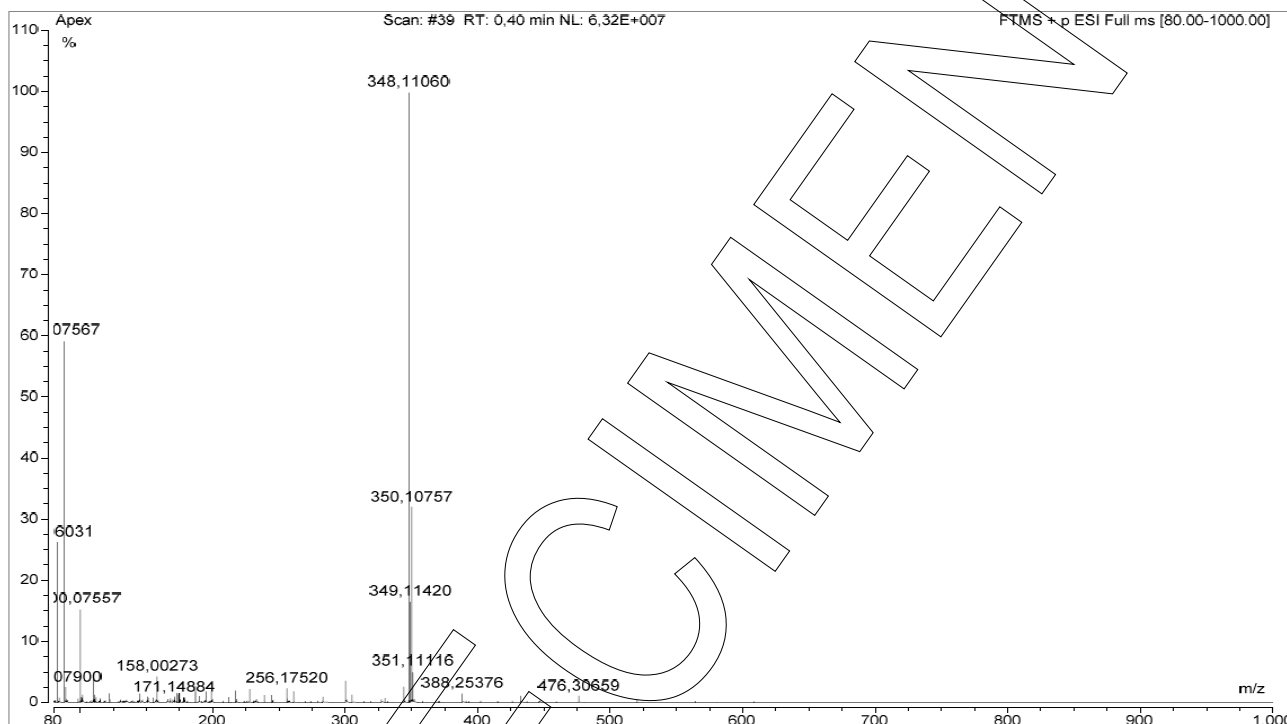



Method	Conditions	Result
IR	Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy	Structure confirmed

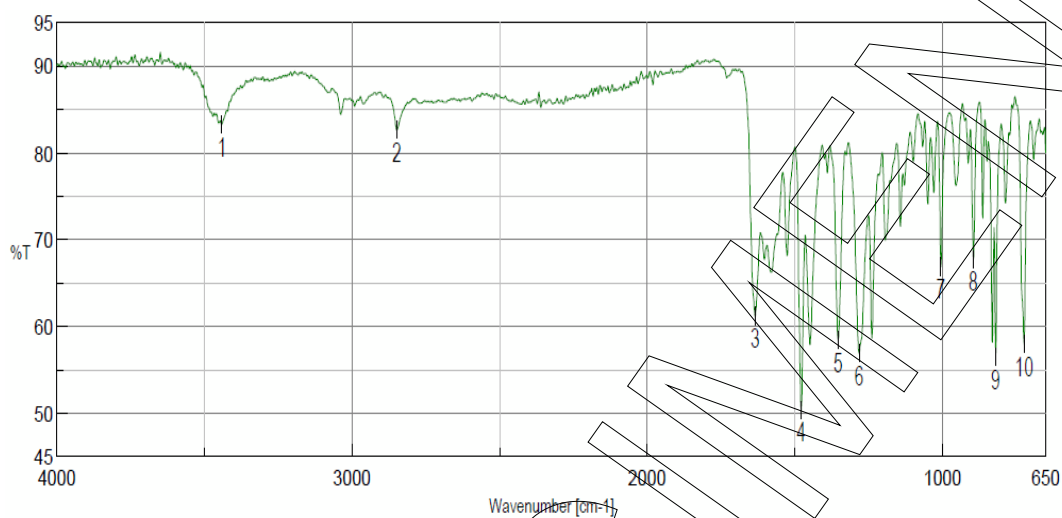

Results of Peak Find		
No.	Position	Intensity
1	3441.35	83.2463
2	2848.35	82.5798
3	1634.38	61.1742
4	1478.17	50.4078
5	1352.82	58.425
6	1282.43	56.9084
7	1004.73	66.846
8	894.809	67.7296
9	818.634	56.4198
10	723.175	57.9474




## Assay

The assay of the reference material was assessed by following analyses.

### Purity by High Performance Liquid Chromatography (HPLC)

HPLC Conditions:	
Column	LiChrospher 60 RP-select B; 5 µm, 125 x 4.0 mm
Column temperature	40 °C
Detector	DAD, 255 nm
Injector	Auto 5.00 µl; 0.073 mg/ml in Acetonitrile/Water 50/50 (v/v)
Flow rate	1.0 ml/min
Phase A	Water, 0.1 % H <sub>3</sub> PO <sub>4</sub>
Phase B	Acetonitrile, 0.1 % H <sub>3</sub> PO <sub>4</sub>
Gradient program	0-10 min A/B 85/15 10-20 min A/B to 50/50 20-25 min A/B 50/50 25-32 min A/B to 85/15 32-40 min A/B 85/15 (v/v)

HPLC chromatogram and peak table

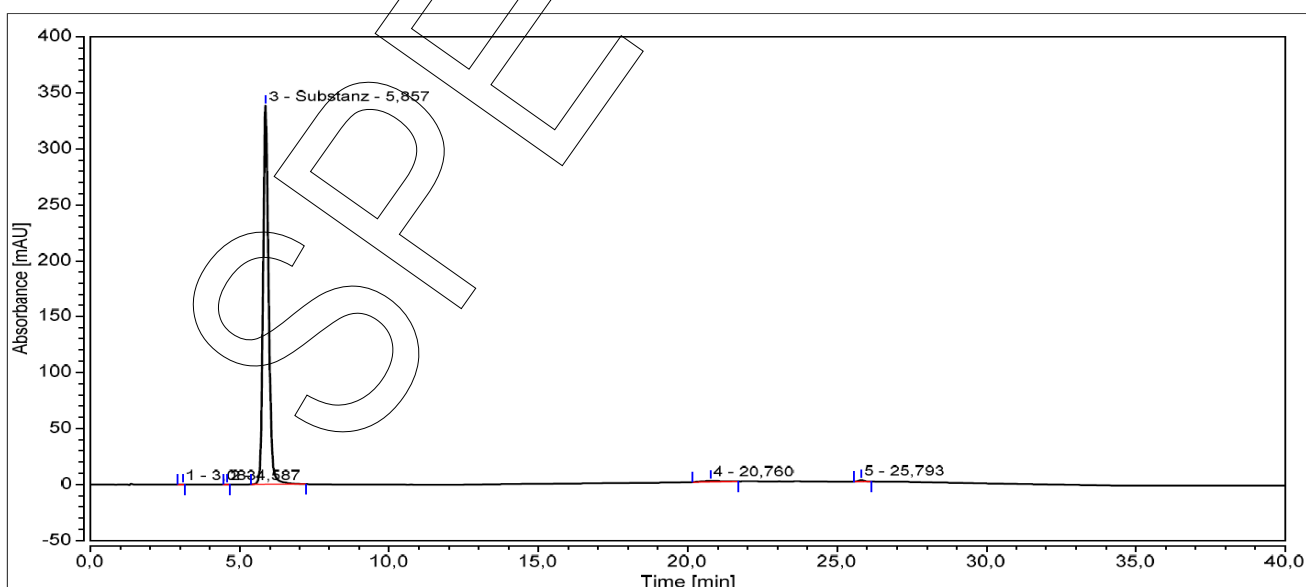



Area percent report - sorted by signal

Pk #	Retention time	Area	Area %
1	3.083	0.012	0.02
2	4.587	0.011	0.02
3	5.857	72.242	98.66
4	20.760	0.656	0.90
5	25.793	0.302	0.41
Totals		73.223	100.00

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

Result (n = 3)

98.66 %, SD = 0.01 %

Volatile content

Water content

Method

Karl Fischer titration

Result (n = 3)

7.36 %, SD = 0.05 %

Residual solvents

Method

<sup>1</sup>H-NMR

Result (n = 1)

No significant amounts of residual solvents were detected (< 0.05 %).



## Final result

**Assay "as is": 91.40 %**

The assay "as is" is assessed by 100% method (mass balance) and is equivalent to the assay based on the not anhydrous and not dried substance respectively.

The calculation of the 100% method follows the formula:

$$\text{Assay (\%)} = (100 \% - \text{volatile contents (\%)}) * \frac{\text{Purity (\%)}}{100 \%}$$

Volatile contents are considered as absolute contributions and purity is considered as relative contribution. Inorganic residues are excluded by additional tests.

## Revision table

Revision	Date	Reason for revision
00	02 Oct 2019	Release of the Certificate of Analysis - initial version

Product warranties for the RM are set out in the terms and conditions of purchase.