

## Certificate of Analysis

### Reference Material - Primary Standard

Product Name: Desmethylcitalopram Hydrochloride 1.0 mg/ml in Methanol (as free base)

Catalogue Number: LGCAMP0242.09-01

Lot Number: 11528

CAS Number: 97743-99-2

Molecular Formula: C<sub>19</sub>H<sub>19</sub>FN<sub>2</sub>O HCl

Molecular Weight: 346.83


Solvent: Methanol

Volume per Ampoule: Not less than 1 ml <sup>1</sup>

Long-term Storage: 2 to 8 °C, dark

Expiry Date: January-2017

Intended Use: The primary aim of this material is for identification, calibration and quantification.

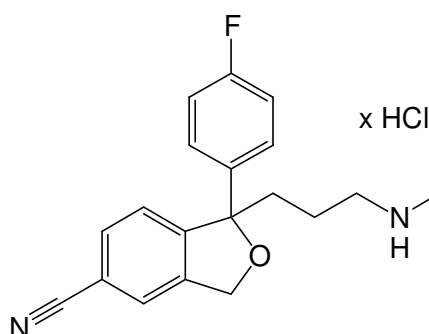


Component	Concentration ("free base")	Uncertainty
see product name	0.895 mg/ml <sup>2</sup>	U = 0.004 mg/ml <sup>3</sup>
Uncertainty of the concentration is expressed as an expanded uncertainty in accordance with ISO 17025 and Guide 34 at the about 95 % level of confidence using a coverage factor of k = 2 and has been calculated by statistical analysis of our production system and incorporates uncertainty of the purity, material density and balance and weighing technique. Concentration based on material weighings and material purity factor (assay of the neat material).		

The solution's concentration and homogeneity are verified by independent method.

LGC certifies that this standard meets the specification stated in this certificate and warrants this product to meet the stated acceptance criteria through the retest date when stored unopened as recommended. Product should be used shortly after opening to avoid concentration changes due to evaporation. Warranty does not apply to ampoules stored after opening.

Release Date:  
Luckenwalde, April 2012

Signed:   
 Dr. Sabine Schröder  
 Unit for Reference Materials

<sup>1</sup> Ampoules are overfilled to ensure a minimum 1 ml volume fill. We advise laboratories to use measured volumes of this standard solution before diluting to the desired concentration.

<sup>2</sup> The value is based on the results of analytical techniques, which calibration and verification was carried out with standards traceable to SI-units. The value is expressed on a "free base" basis.

The concentration with its uncertainty is valid in the range between 19 °C and 25 °C.

The identity is verified by data from international scientific literature.

Gravimetrically prepared using qualified balances calibrated annually by accredited calibration service. Calibration verification performed daily prior to use utilizing weights traceable to SI via other mass standards.

<sup>3</sup> The uncertainty "U" is the expanded uncertainty estimated in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM). It is corresponding to a level of confidence of about 95 %. Standard uncertainties are indicated with "u".

Additional information	
Concentration ("as is")	1.000 mg/ml

Verification of Concentration and Homogeneity				
Lot Number	Verified Concentration (mg/ml)		% RSD - Homogeneity	
	Result	Acceptance Criteria	Result	Acceptance Criteria
11528	0.891	± 3 %	1.640	≤ 3 %
Concentration verified by HPLC				

Solution Standard Assay Parameters		External Calibration (100 % amount)	
Analysis Method	HPLC		
Column:	60 RP Select B, 5 µm, 125 x 4 mm	Number of Measurements:	6
Injector:	Auto; 3 µl; 1.0 mg/ml in Methanol		
Flow:	1.0 ml/min, 40 °C	Detector:	240 nm
Conditions:	mob. Phase A: Water + 0.1 % H <sub>3</sub> PO <sub>4</sub> , mob. Phase B: Acetonitrile + 0.1 % H <sub>3</sub> PO <sub>4</sub> 0-8 min A/B 70/30, 8-11 min A/B to 50/50, 11-13 min A/B to 70/30, 13-20 min A/B 70/30 (v/v)		

Neat Material Data		
Product Name:	Desmethylcitalopram Hydrochloride	
CAS Number:	97743-99-2	
Molecular Formula:	C <sub>19</sub> H <sub>19</sub> FN <sub>2</sub> O HCl	
Molecular Weight:	346.83	
Compound Lot:	7790	
Test	Method	Result
Melting Point (°C)*	SOP 06-010	160 °C
<sup>1</sup> H-NMR Spectrum*	SOP 06-053	conform / complies to structure
IR Spectrum*	SOP 06-036	conform / complies to structure
Mass Spectrum (ESI)*	SOP 06-022	conform / complies to structure
<b>Assay by quantitative NMR (free base)*</b>	<b>Quant. NMR</b>	<b>86.93 %</b>
The expanded uncertainty according to the assay is U = 0.36 % (about 95 % level of confidence using a coverage factor of k = 2).		
Assay by quantitative NMR ("as is")*	97.14 %	

\*: Validated method performed by ISO/IEC 17025 accredited testing lab

The assay of the neat material is verified by the 100 % method using HPLC, corrected with water (KFT) and residual solvents.




## I. Identity

The identity of the reference substance (neat material) was established by the following analyses.

### Ia. <sup>1</sup>H-NMR Spectrum


Conditions: 400 MHz, DMSO-d<sub>6</sub>

The structure is confirmed with the signals of the spectrum and their interpretation.

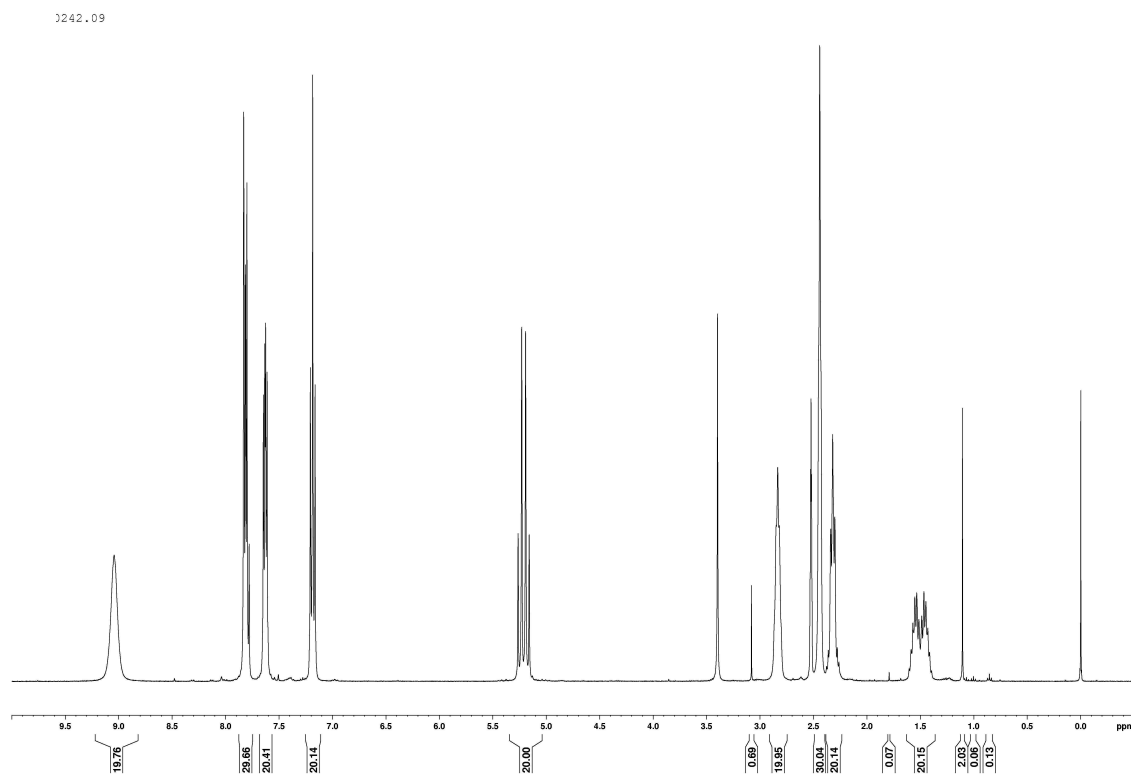

**1b. Mass Spectrum**

Method: 4.5 kV ESI; vaporization temperature: 200 °C, direct inlet

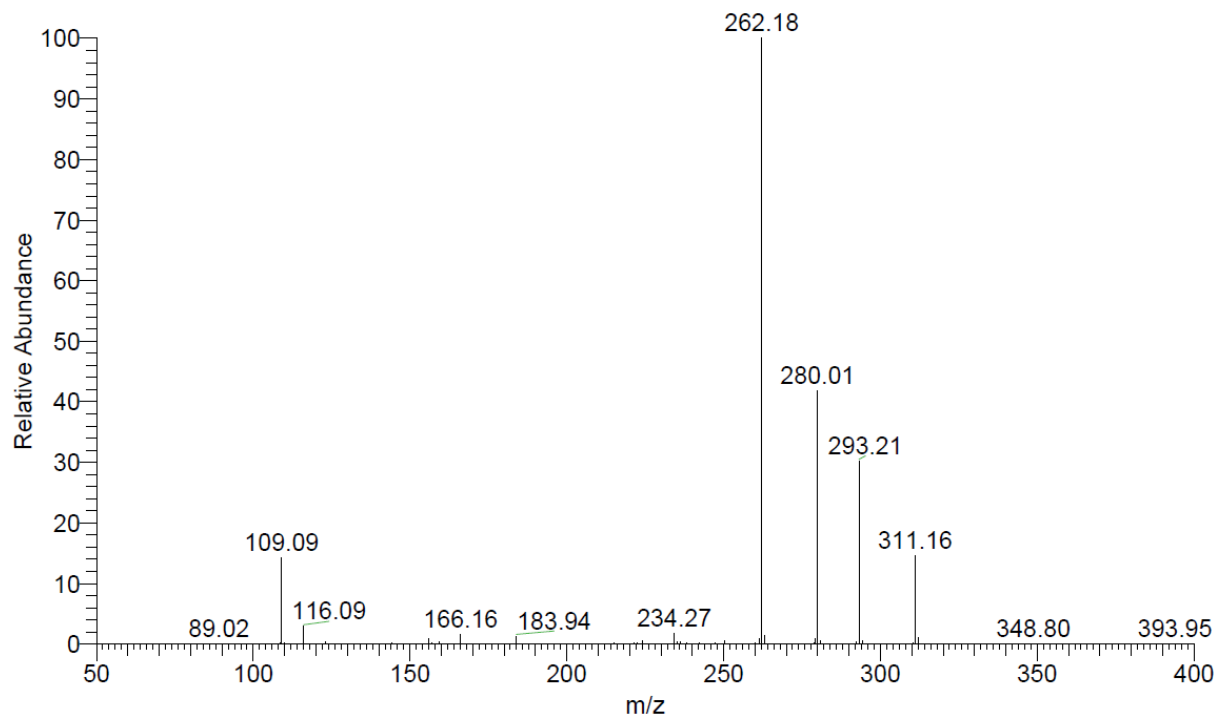


m/z	fragments (M = free base)
311.16	[ MH ]
280.01	[ M – CH <sub>3</sub> NH ]
262.18	[ MH – F – CH <sub>3</sub> NH ]

The signals of the mass spectrum and their interpretation are consistent with the structural formula.

## lc. IR Spectrum

Method: attenuated total reflection fourier transform infrared (ATR-FTIR) spectroscopy

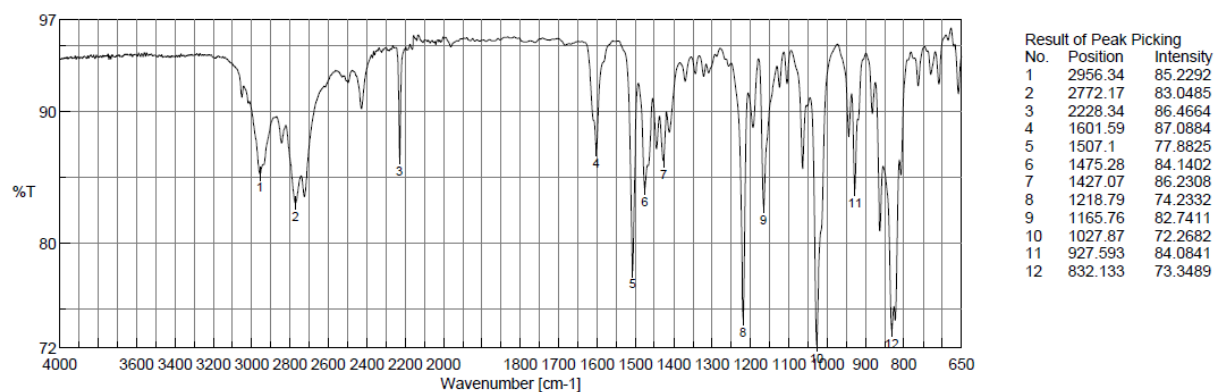


The signals of the IR spectrum and their interpretation are consistent with the structural formula.

## ld. Melting Point

160 °C


## le. UV Spectrum

Method: HPLC (DAD-detection)

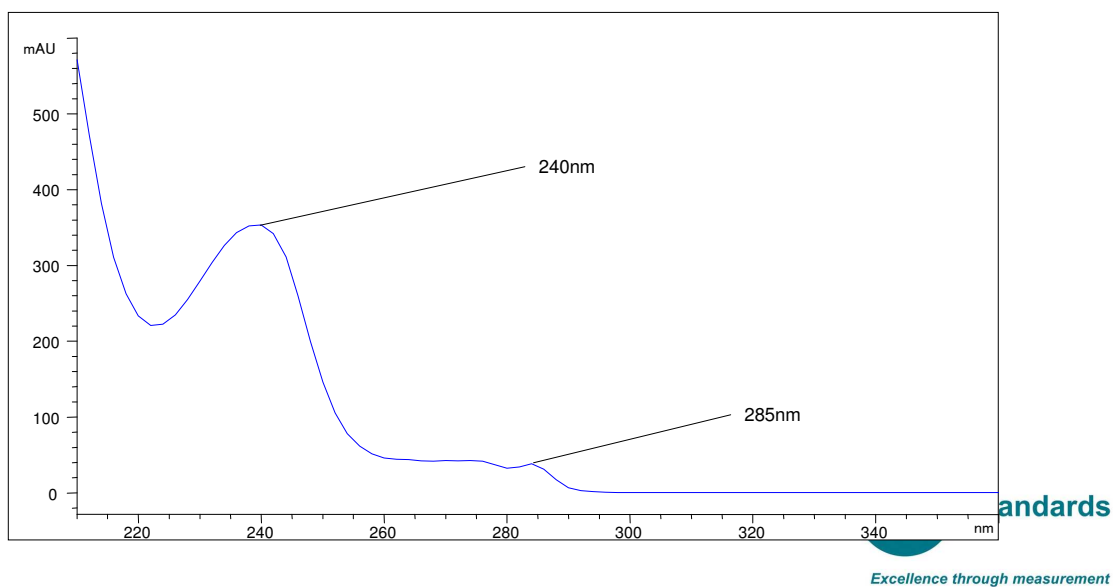

## II. Assay by quantitative NMR spectroscopy

The assay of the reference substance was established by quantitative NMR spectroscopy using DMSO-d<sub>6</sub> as the solvent and with Maleic acid (certified reference material, signal 5.90 – 6.65 ppm, 2 H) as internal standard.

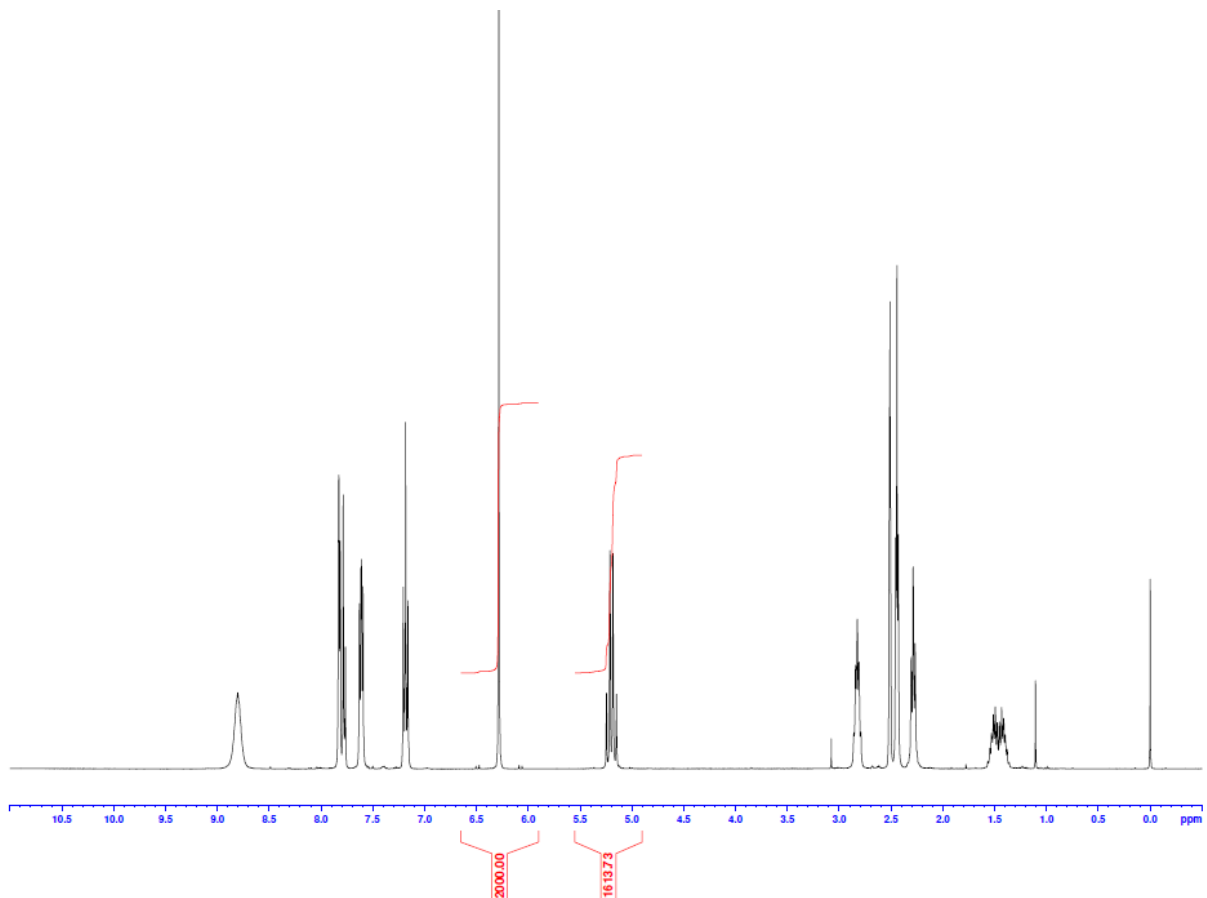


### Results:

Average	97.14 %
Number of results	n=6
Uncertainty U (expanded)	0.40 %

### III. Purity

#### IIIa. High Performance Liquid Chromatography (HPLC)

The purity of the reference substance (neat material) was analysed by high performance liquid chromatography (HPLC).

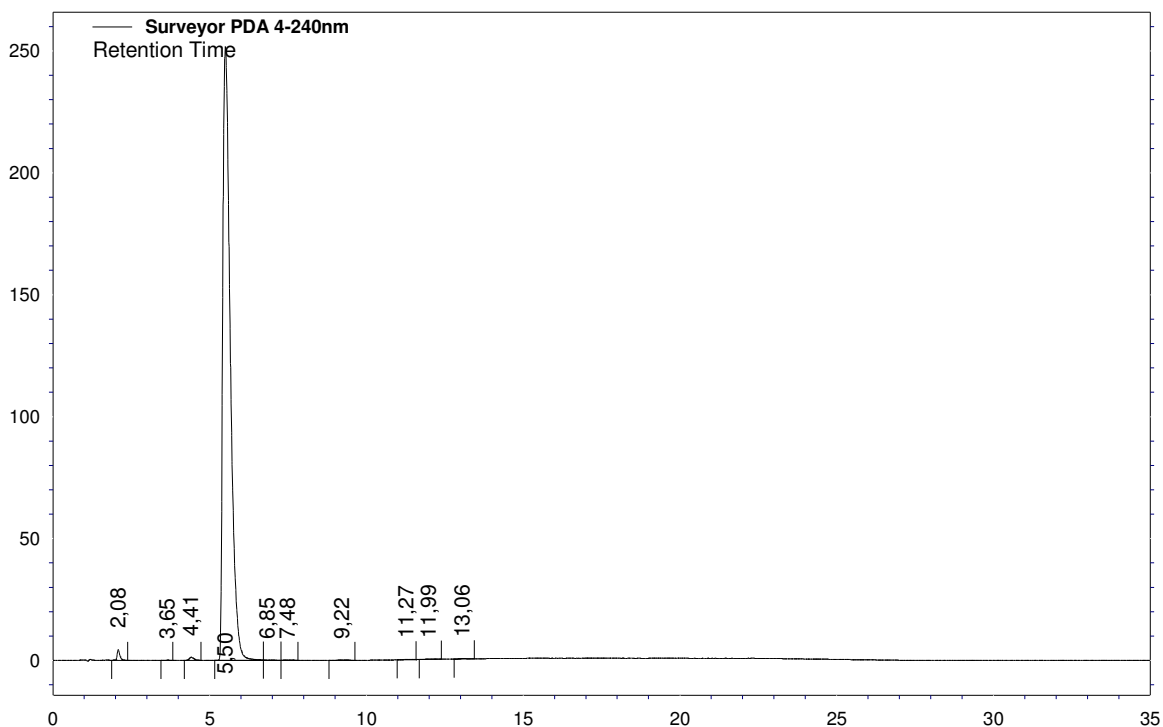

#### Area Percent Report - Sorted by Signal

Pk #	Retention Time	Area	Area %
1	2.08	25682	0.60
2	3.65	1224	0.03
3	4.41	14159	0.33
4	5.50	4198949	98.64
5	6.85	3447	0.08
6	7.48	2639	0.06
7	9.22	3392	0.08
8	11.27	1487	0.03
9	11.99	2301	0.05
10	13.06	3413	0.08
Totals		4256693	100.00



For the calculation the system peaks were ignored. The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %.

**HPLC Conditions:**

<b>Column:</b>	<b>Conditions:</b>	<b>Detector:</b>	<b>Injector:</b>
RP 60 Select B 5 µm, 125 x 4 mm	1.0 ml/min, 40 °C 0-7 min Water/Acetonitrile 70/30 7-12 min Water/Acetonitrile to 65/35 12-20 min Water/Acetonitrile 65/35 20-25 min Water/Acetonitrile to 70/30 25-35 min Water/Acetonitrile 70/30 (v/v); 0.1 % H <sub>3</sub> PO <sub>4</sub>	DAD 240 nm	Auto 6 µl; 0.0652 mg/ml in Water/Acetonitrile 50/50 (v/v)

**Results:**

**Arithmetic mean (n=3)**      98.65 %

**IIIb. Water Content**

Method: coulometric Karl Fischer titration

**Results:**

**Arithmetic mean (n=3)**      0.33 % (mass fraction)

**IIIc. Residual Solvents**

Method: <sup>1</sup>H-NMR

Result: 0.58 % *tert*-Butyl methyl ether  
0.05 % *n*-Hexane



#### IV. Stability and Homogeneity

Accelerated stability studies indicate no significant instability. The given validity period is based on this data. This is backed up by historical data over the range of several years for the neat substance. Homogeneity assured by validated process of preparation (incl. ampoulation), verified by homogeneity testing (HPLC).

#### V. Further Information

##### General

For laboratory use only. Not suitable for human or animal consumption.

This material conforms to the characteristics of a primary standard as described within ISO Guide 30 (Terms and definitions used in connection with reference materials).

The certified values quoted in this certificate are LGC's best estimate of the true values within the stated uncertainties and based on the techniques described in this certificate.

##### Handling of the RM

Before usage of the RM, it should be allowed to warm to room temperature. The concentration with its uncertainty is guaranteed in the range between 19 °C and 25 °C. The uncertainty accounts for the temperature-dependent density in this range.

##### Quality Control Assessment

The product quality is controlled by regularly performed quality control tests (retests).

Revision	Date	Reason for Revision
00	April 2012	Release of the Lot – initial version
01	March 2013	Copyright added