



Reference Materials for Residue Analysis

## **Gravimetric Certificate**

ISO Guide 34 Reference Material

Product Identification

Article Code: DRE-XA14075000CY Article Name: epsilon-HCH Formula: C6H6Cl6

Mol. Weight: 290.8 CAS No.: 6108-10-7 Lot Number:

G120350CY

**Expiry Date:** 

28.02.2022

**Storage Temperature:** 

20°C ± 4°C

Storage and handling: The RM should be stored in the original sealed bottle at the temperatur given above. After use the bottle should be tightly closed and protected from moisture and light. The expiry date is valid for original sealed bottles under recommended storage conditions only.

Compound Name:

Lot: 119222 Purity: 99.9%

Weight (mg): 48.048

epsilon-HCH Solvent: Cyclohexane

Solvent Lot: D5M005155N45 Exact Quantity (ml):

480.00

Concentration:

100.00 mg/l

Expanded Uncertainty U=

2.31 mg/l

The uncertainty of this standard is calculated in accordance with the ISO Guide 34 and EURACHEM/CITAC Guide - Quantifying Uncertainty in Analytical Measurement, Second Edition. The expanded uncertainty is U(exp) = u(RM) x k, where k is the coverage factor at the 95% confidence level (k=2). Uncertainty u(RM) is based on the combination of the uncertainties associated with each individual operation involved in the analysis of the product: u(RM) = vu(char)² + u(bb)² + u(lts)² + u(sts)² ; u(char) is the uncertainty of characterisation; u(bb) uncertainty of homogeneity test; u(lts) uncertainty of stability test long-term; u(sts) uncertainty of stability test short-term. u(lts) and u(sts) are not included in the calculation as the stability statement is based on real evidence opposed to simulation. Minimum sample: 1 ml is recommended as the minimal sample amount. If less material is used, it is recommended to increase the certified uncertainty by a factor of two for half sample and a factor of four for a quarter of sample.

Intended use: Use this RM as calibrant for chromatography or any other analytical technique.

## Analytical Data

Traceability of chromatography: To the International System of Units (SI).

Intrument: Detection:

FID

Optima-5MS, 0.25 µm, 0.25 mm

Initial Temp:

60°C for 5 min

1 µl

Ret.Time:

1.0 ml/min 16.61 min

End Temp: Gradient:

280°C for 1 min 15°C/min

Column:

Inj.-Vol.:

Traceability: The balances used are calibrated with weights traceable to the national standards (DKD).

Calibrated class A glassware is used for volumetric measurements.

Certificate Revision 1

Certified on: Certified by: 28.02.2017

M. Beck M. Beck

The LGC Labor GmbH, accreditated by DAkkS as indicated by the accreditation number D-RM-19883-01 & D-PL-19883-01, has shown competence based on ISO Guide 34:2009 with relevant parts of DIN EN ISO/IEC 17025:2005 for production of certified reference materials in form of organic pure substances and in form of single and multi-component solutions of organic pure substances. Data File L:\GERÄTE ...D2\2016\2016KW45\KW2016KW45-5A 2016-11-11 14-26-47\14075000-00011.D Sample Name: G120350CY

FL90.53 B Acq. Operator : FID2 Seq. Line: 29

Acq. Instrument : GC-FID-2 Location : Vial 41

Injection Date : 12.11.2016 6:19:27 Uhr Inj: Inj Volume: 1.000 µl

: C:\CHEM32\1\DATA\2016KW45\KW2016KW45-5A 2016-11-11 14-26-47\PESK.M Acq. Method


Last changed : 04.11.2015 11:25:42 Uhr by FID2

Analysis Method: L:\GERÄTE BACKUP\FID2\NEUE METHODEN\PESK.M

: 27.02.2017 11:39:18 Uhr Last changed (modified after loading)

Method Info : pesk

Sample Info : epsilon-HCH

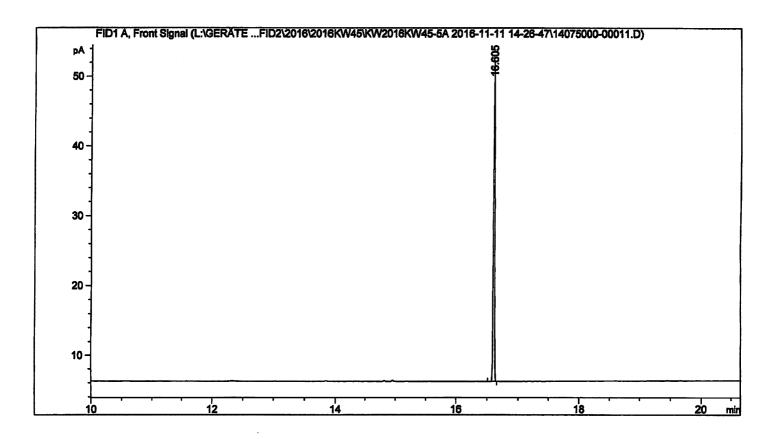

## Area Percent Report

Sorted By Signal

1.0000 Multiplier: : Dilution: : 1.0000

Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A, Front Signal

Peak RetTime Type Width Area Height Area [min] [min] [pA\*s] [pA] \_\_\_\_ 45.89879 100.0000 1 16.605 BB 0.0227 65.66171

Totals: 65.66171 45.89879