



Mikromol™



# Certificate of Analysis

ISO 17034

## Reference Material

### Product name

Cycloserine

### Product code

MM3028.00

### CAS number

68-41-7

### Molecular weight

102.09

### Molecular formula

C<sub>3</sub>H<sub>6</sub>N<sub>2</sub>O<sub>2</sub>

### Lot number

G1019085

### Appearance


white solid

### Melting point

133 °C (dec)

### Long-term storage

-18 °C, dark



Assay<sup>1</sup> "as is"  
98.8 %

Uncertainty<sup>2</sup> U  
0.4 %

**Intended Use:** Use for identification and quantification. The assay is verified by a second testing method. Due to the homogeneity studies, the minimum amount of sample to be used is 10mg.

Date of shipment:

**04 Nov 2019**

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **two years** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

|                     |                          |  |                 |
|---------------------|--------------------------|--|-----------------|
| <b>Release by:</b>  | <b>Date of Release:</b>  |  | Product Release |
| Dr. Sabine Schröder | Luckenwalde, 02 Oct 2019 |  |                 |

<sup>1</sup> Calibration and verification were carried out using standards traceable to SI-units. The value is expressed on an "as is" basis.

<sup>2</sup> The uncertainty "U" is the expanded uncertainty of the testing method for the assigned value estimated in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM). It corresponds to a level of confidence of about 95%. Coverage factor k = 2.



## Important product information

This RM is intended for laboratory use only and is not suitable for human or animal consumption.

This RM conforms to the characteristics of a primary standard as described in the ICH Guidelines. The values quoted in this Certificate of Analysis are the producer's best estimate of the true values within the stated uncertainties and based on the techniques described in this Certificate of Analysis. The production of this RM was undertaken in accordance with the requirements of ISO 17034. The identity is verified by data from international scientific literature.

## Storage and handling

Before usage of the RM, it should be allowed to warm to room temperature. No drying is required, as assigned values are already corrected for the content of water and other volatile materials.

## Further content

Assigned value

Purity

Identity

Stability and homogeneity

Revision table



## Assigned value

**Assay "as is": 98.84 %; U = 0.42 %**


The assay "as is" is assessed by quantitative NMR spectroscopy and is equivalent to the assay based on the not-anhydrous and not-dried substance. The assay is verified by 100% method (mass balance).

The verified result lies inside our acceptance criteria, i.e. less than 1.0 % difference to assay assigning technique.

For quantitative applications, use the assay as a calculation value on the "as is basis". The uncertainty of the assay can be used for estimation/calculation of measurement uncertainty.

| Method 1: Value assigning technique - quantitative NMR spectroscopy |   |
|---|---|
| Conditions  | 400 MHz, DMSO-d <sub>6</sub>  |
| Internal standard   | 1,3,5-Trimethoxybenzene (certified reference material), signal 5.7 - 6.5 ppm, 3 H |
| Result (mass fraction, n = 6)                                       | 98.84 %; U = 0.42 %   |

Quantitative NMR spectrum

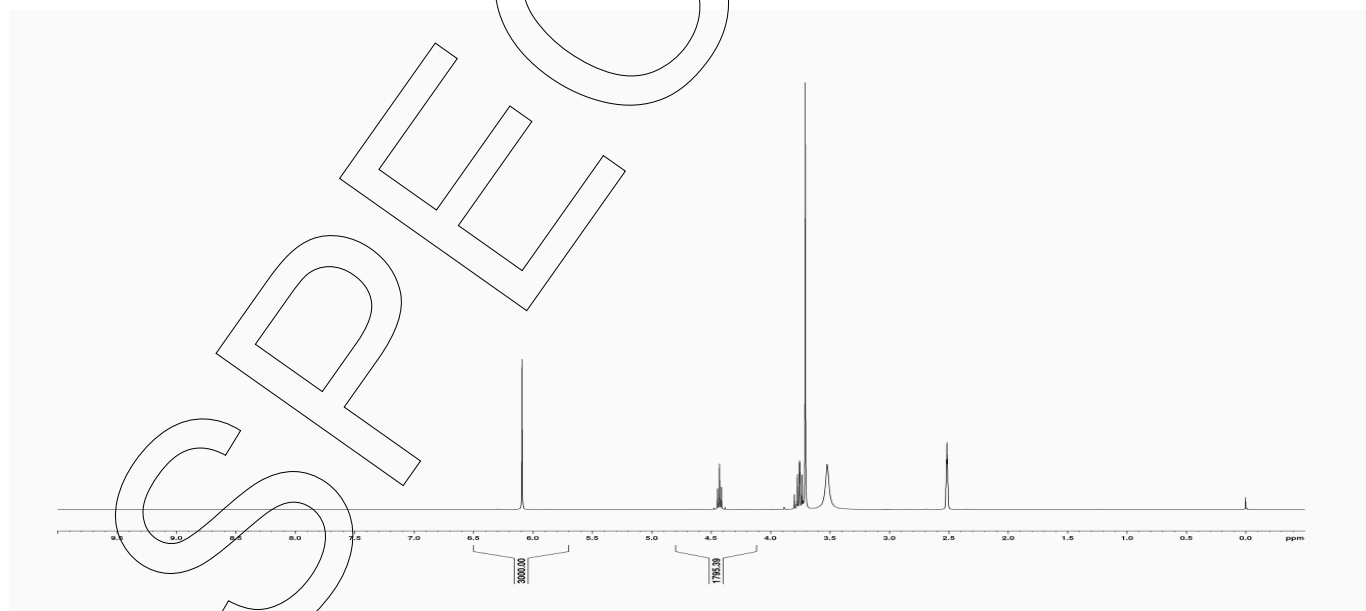



## Method 2: Value verifying technique - 100% method

**100% method (mass balance) with chromatographic purity by HPLC**

**Result** 99.75 %

The calculation of the 100% method follows the formula:

$$\text{Assay (\%)} = (100 \% - \text{volatile contents (\%)}) * \frac{\text{Purity (\%)}}{100 \%}$$

Volatile contents are considered as absolute contributions and purity is considered as relative contribution.  
Inorganic residues are excluded by additional tests.


## Purity

### Purity by High Performance Liquid Chromatography (HPLC)

| HPLC Conditions:   |   |
|--------------------|---|
| Column             | Discovery HS F5; 3 µm, 150 x 4.0 mm   |
| Column temperature | 40 °C   |
| Detector           | DAD, 220 nm   |
| Injector           | Auto 3.00 µl; 0.181 mg/ml in Acetonitrile/Water 50/50 (v/v)                                     |
| Flow rate          | 1.0 ml/min  |
| Phase A            | Water, 0.1 % H <sub>3</sub> PO <sub>4</sub>   |
| Phase B            | Acetonitrile, 0.1 % H <sub>3</sub> PO <sub>4</sub>  |
| Gradient program   | 0-6 min A/B 24/76<br>6-9 min A/B to 70/30<br>9-11 min A/B to 24/76<br>11-20 min A/B 24/76 (v/v) |



HPLC chromatogram and peak table

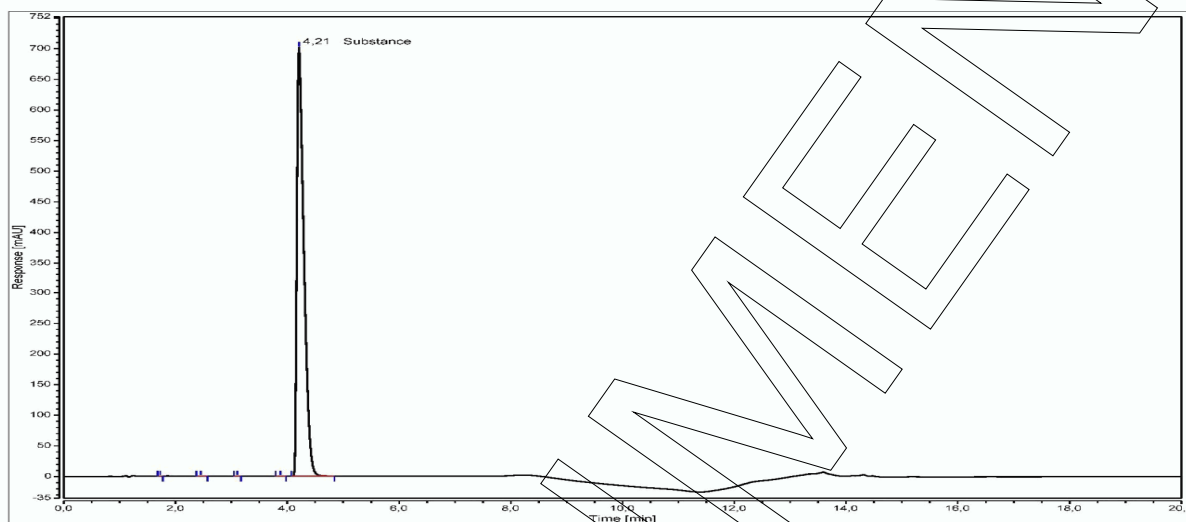

Area percent report - sorted by signal

| Pk #   | Retention time | Area    | Area % |  |
|--------|----------------|---------|--------|--|
| 1      | 1.728          | 0.010   | 0.01   |  |
| 2      | 2.455          | 0.013   | 0.01   |  |
| 3      | 3.102          | 0.014   | 0.01   |  |
| 4      | 3.875          | 0.014   | 0.01   |  |
| 5      | 4.208          | 101.388 | 99.95  |  |
| Totals |                | 101.439 | 100.00 |  |

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

Result (n = 6)

99.95 %; U = 0.18 %



## Volatile content

### Water content

|                       |                        |
|-----------------------|------------------------|
| <b>Method</b>         | Karl Fischer titration |
| <b>Result</b> (n = 3) | 0.20 %*; SD = 0.01 %   |

\*not accredited testing method

### Residual solvents

|                       |  |
|-----------------------|--|
| <b>Method</b>         | <sup>1</sup> H-NMR   |
| <b>Result</b> (n = 1) | No significant amounts of residual solvents were detected (< 0.05 %).* |

\*not accredited testing method

## Inorganic residues

**Method:** Sulphated ash, EP 8.7 (2.4.14)\*

According to the available data, the presence of inorganic impurities in the reference material other than those detectable by sulphated ash is highly unlikely. Inorganic residues can be excluded by results of the sulphated ash. Therefore, no assay correction was performed for inorganic impurities.

\*not accredited testing method




Mikromol<sup>TM</sup>

## Identity


The identity is assessed by ISO/IEC 17025 accredited testing methods.

| Method             | Conditions                | Result              |
|--------------------|---------------------------|---------------------|
| <sup>1</sup> H-NMR | 400 MHz, D <sub>2</sub> O | Structure confirmed |

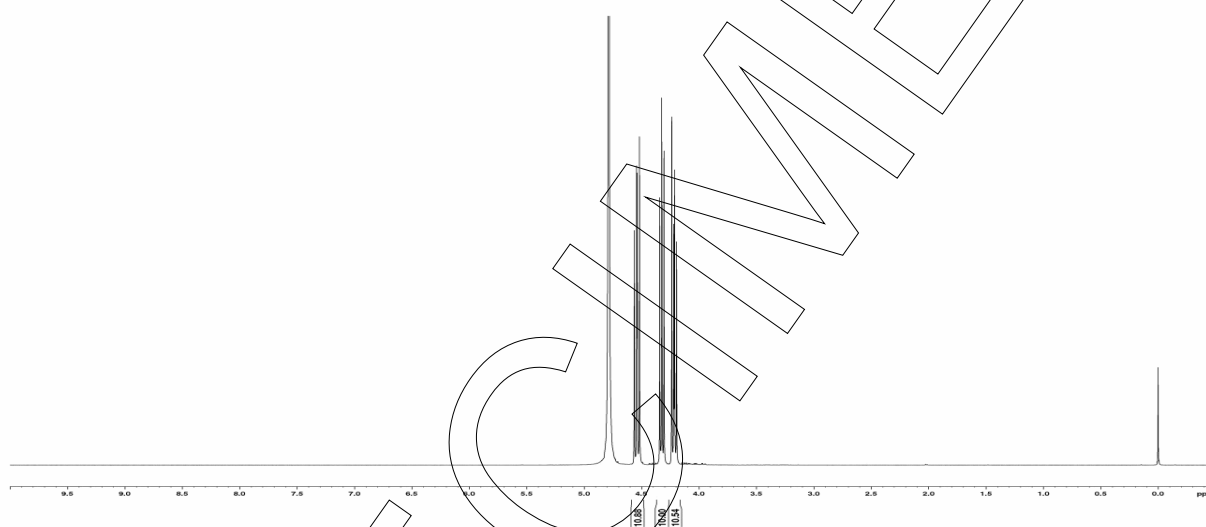




| Method | Conditions   | Result              |
|--------|--|---------------------|
| MS     | 3.5 kV ESI+; capillary temperature: 269 °C<br>Theoretical value: 103.05020 | Structure confirmed |

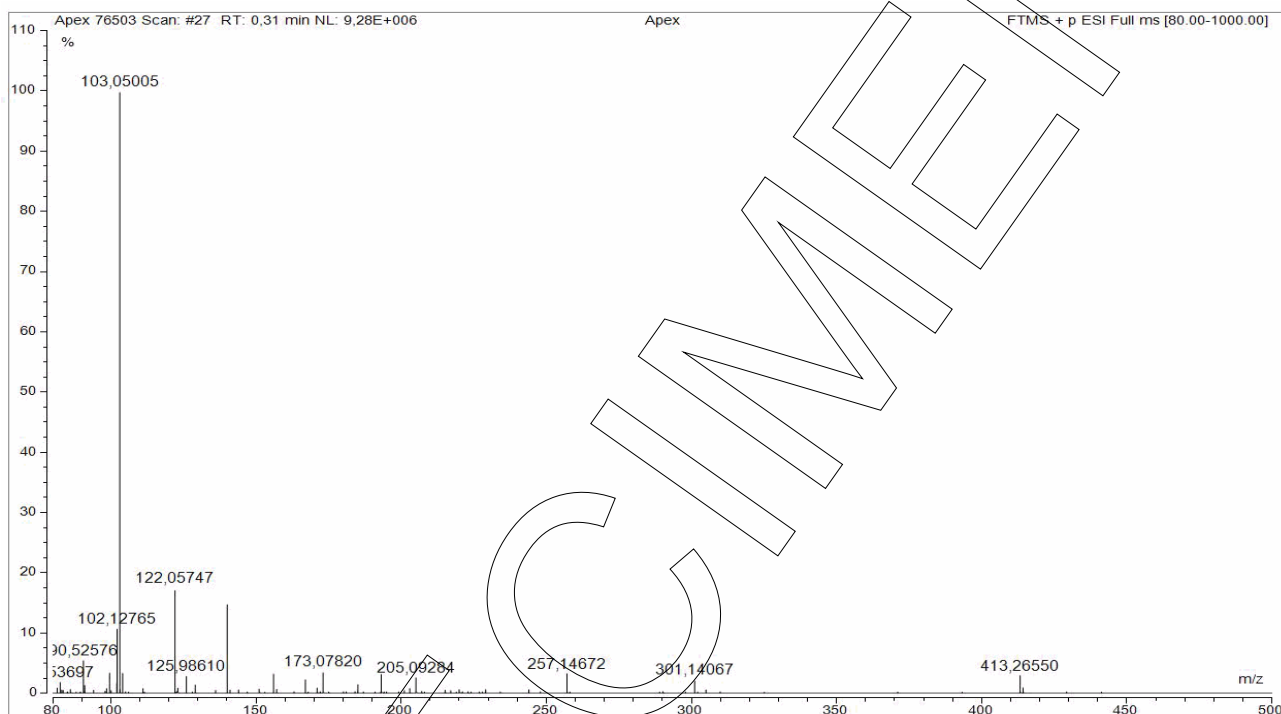





| Method | Conditions   | Result              |
|--------|--|---------------------|
| IR     | Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy | Structure confirmed |

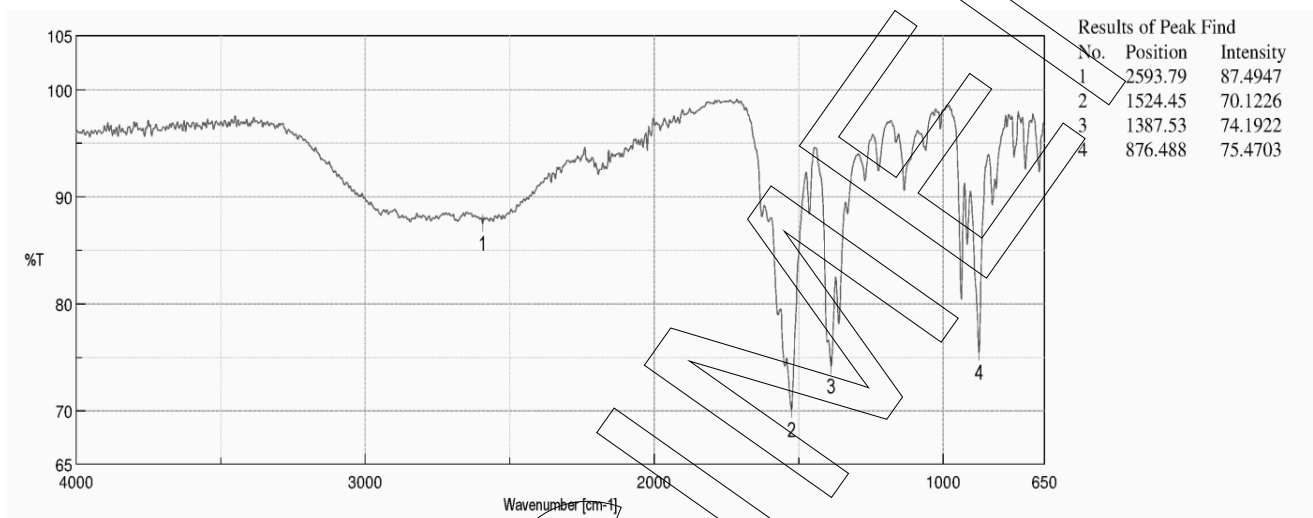

## Stability and homogeneity

Accelerated stability studies indicate no significant instability. The given validity period is based on this data. This is backed up by additional stability testing and historical data over the range of several years.

RM quality is controlled by regularly performed quality control tests (re tests). Homogeneity assured by qualified process of preparation and verified by homogeneity testing.

## Revision table

| Revision | Date        | Reason for revision                                      |
|----------|-------------|--|
| 00       | 02 Oct 2019 | Release of the Certificate of Analysis - initial version |

Product warranties for the RM are set out in the terms and conditions of purchase.