

Certificate of Analysis

ISO 9001

Reference Material

Product name

3,4-Bis(cyclopropylmethoxy)-N-(3,5-dichloropyridin-4-yl)benza mide


Product code Lot number MM3618.04 992599

CAS number Appearance 1391052-24-6 white solid

Molecular weight Melting point (DSC)

407.29 210 °C

 $\begin{tabular}{ll} \textbf{Molecular formula} & \textbf{Long-term storage} \\ C_{20}H_{20}Cl_2N_2O_3 & 2 to 8 \, ^{\circ}\text{C}, dark \\ \end{tabular}$

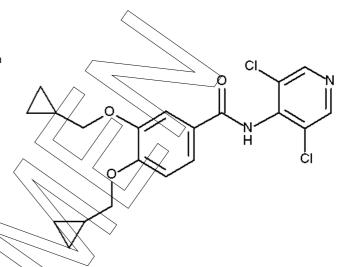

Assay "as is'

Date of shipment: 05 Feb 2020

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **one year** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

Release by:

Date of Release:

Dr. Sabine Schröder

Luckenwalde, 12 Aug 2019


Product Release



Product information

For laboratory use only. Not suitable for human or animal consumption.


Before usage of the RM, it should be allowed to warm to room temperature. No drying required, as the certified value is already corrected for the content of water and other volatile materials.

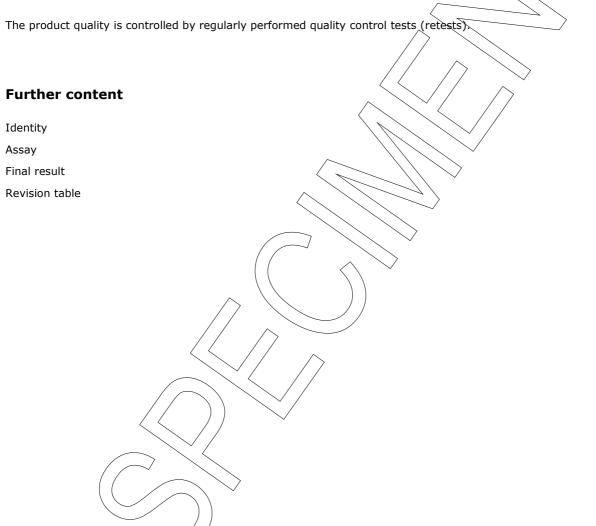




Identity


The identity of the reference material was established by following analyses.

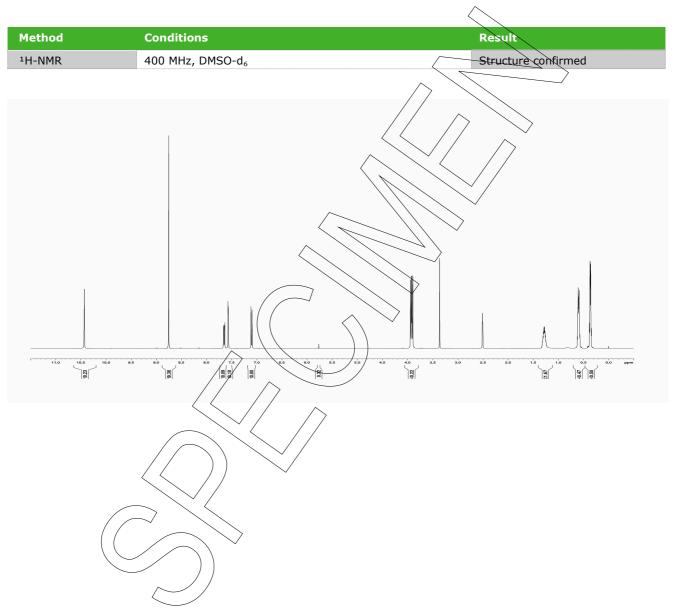



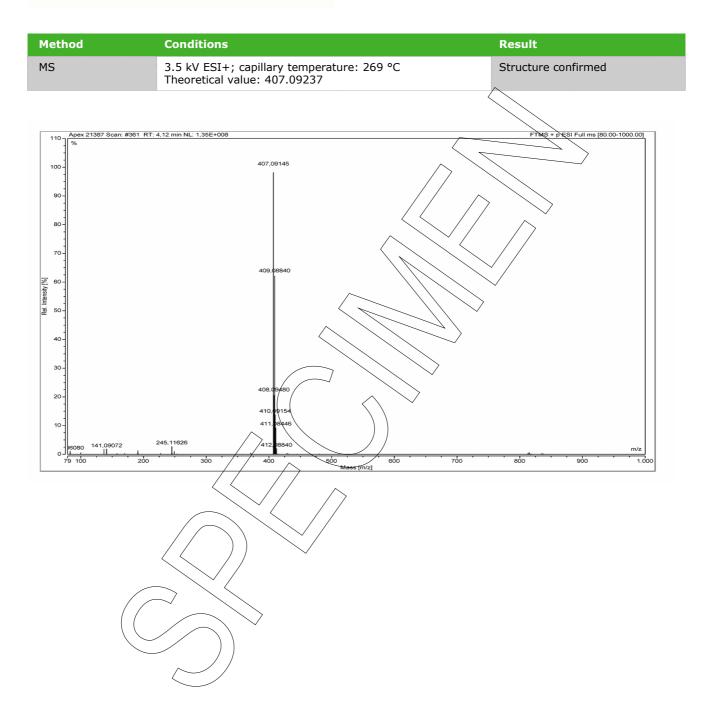



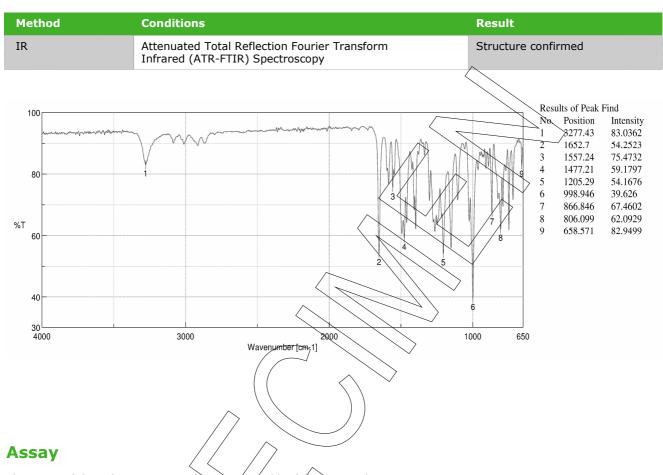

The assay of the reference material was assessed by following analyses.

Purity by High Performance Liquid Chromatography (HPLC)


HPLC Conditions:	
Column	Kinetex Phenyl-Hexyl; 1.7 μm, 100 x 2.1 mm
Column temperature	40 °C
Detector	DAD, 210 nm
Injector	Auto 1 μl; 0.050 mg/ml in Acetonitrile
Flow rate	0.5 ml/min
Phase A	Water, 0.1 % HCOOH
Phase B	Acetonitrile, 0.1 % HCOOH
Gradient program	0-1 min A/B 98/2
	1-4 min A/B to 2/98
	4-5 min A/B to 98/2
	5-6 min A/B 98/2 (v/v)

LGC GmbH, Louis-Pasteur-Str. 30, D-14943 Luckenwalde, Germany

Page 5/7 MM3618.04 Lot number 992599



HPLC chromatogram and peak table

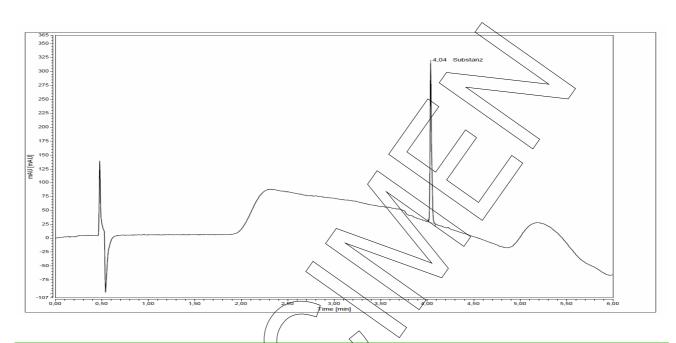

Area percent report - sorted by signal			
Pk #	Retention time	Area	Area %
1	4.037	5.4423	100.00
Totals		5,4423	100.00

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

Result (n = 3) 100.00 %; SD < 0.01 %



Volatile content

Water content		^
Method	Karl Fischer titration	
Result (n = 3)	0.08 %; SD = 0.01 %	

Residual solvents	
Method	¹H-NMR
Result (n = 1)	No significant amounts of residual solvents were detected (< 0.05 %).

Final result

Assay "as is": 99.92 %

The assay "as is" is assessed by 100% method (mass balance) and is equivalent to the assay based on the not anhydrous and not dried substance respectively.

The calculation of the 100% method follows the formula:

Purity (%) Assay (%) = (100 % - volatile contents (%)) 100 %

Volatile contents are considered as absolute contributions and purity is considered as relative contribution. Inorganic residues are excluded by additional tests.

Revision table

Revision	Date	Reason for revision
00	12 Aug 2019	Release of the Certificate of Analysis - initial version

Product warranties for the RM are set out in the terms and conditions of purchase.

Page 7/7 MM3618.04 Lot number 992599