

Reference Material

Product Name
Pesticide-Mix 102 50 µg/mL in Acetonitrile

Product Code
DRE-LA18000102AL

Lot Number
G1012775AL

Format
Multicomponent Solution

Expiry Date
31 May 2023

Storage Temp
20°C ± 4°C

This certificate is designed in accordance with ISO 17034 and ISO Guide 31. This reference material (RM) was designed, produced and verified in accordance with ISO/IEC 17025, ISO 17034 and a registered quality management system ISO 9001.

REFERENCE MATERIAL CERTIFICATE

ISO 17034

| Compound Name | CERTIFIED | | CAS | Lot Number | Purity (%) | Amount (mg) | RT (min) |
|--|-----------------------|--------------------------------|------------|------------|------------|-------------|----------|
| | Concentration (µg/mL) | Expanded Uncertainty U (µg/mL) | | | | | |
| alpha-HCH | 50.00 | 2.51 | 319-84-6 | 120435 | 98.1 | 5.097 | 28.15 |
| Hexachlorobenzene | 50.02 | 2.51 | 118-74-1 | G120431 | 99.9 | 5.007 | 28.54 |
| beta-HCH | 50.03 | 2.51 | 319-85-7 | G138918 | 98.6 | 5.074 | 29.20 |
| gamma-HCH | 50.02 | 2.51 | 58-89-9 | G167195 | 98.8 | 5.063 | 29.51 |
| Heptachlor | 49.97 | 2.50 | 76-44-8 | 41025 | 99.0 | 5.047 | 32.52 |
| Alachlor | 50.02 | 2.51 | 15972-60-8 | 984292 | 97.3 | 5.141 | 32.58 |
| Aldrin | 50.03 | 2.51 | 309-00-2 | G991490 | 98.2 | 5.095 | 33.88 |
| Metolachlor | 50.03 | 2.51 | 51218-45-2 | 126892 | 97.9 | 5.110 | 33.99 |
| Chlorpyrifos | 49.97 | 2.50 | 2921-88-2 | 175254 | 99.6 | 5.017 | 34.16 |
| trans-Heptachlor-endo-epoxide (isomer A) | 49.96 | 2.50 | 28044-83-9 | 124021 | 99.1 | 5.041 | 35.54 |
| alpha-Endosulfan | 50.03 | 2.51 | 959-98-8 | G150002 | 98.1 | 5.100 | 36.71 |
| Dieldrin | 49.96 | 2.50 | 60-57-1 | 126109 | 99.9 | 5.001 | 37.68 |
| Endrin | 50.01 | 2.51 | 72-20-8 | 126168 | 96.5 | 5.182 | 38.44 |
| beta-Endosulfan | 49.99 | 2.50 | 33213-65-9 | G139276 | 99.6 | 5.019 | 38.75 |
| 4,4'-DDD | 49.98 | 2.50 | 72-54-8 | 120073 | 98.7 | 5.064 | 39.12 |
| 2,4'-DDT | 50.01 | 2.51 | 789-02-6 | 123981 | 97.6 | 5.124 | 39.29 |
| 4,4'-DDT | 49.97 | 2.50 | 50-29-3 | 985808 | 97.8 | 5.109 | 40.49 |

The producer certifies that this reference material meets the specification stated in this certificate until the expiry date, provided it is stored unopened at the recommended temperature herein. Product warranties for this reference material are set out in the terms and conditions of purchase.

CERTIFIED BY


D. Schmid

CERTIFIED ON

31 May 2019

D. Schmid

RM Release

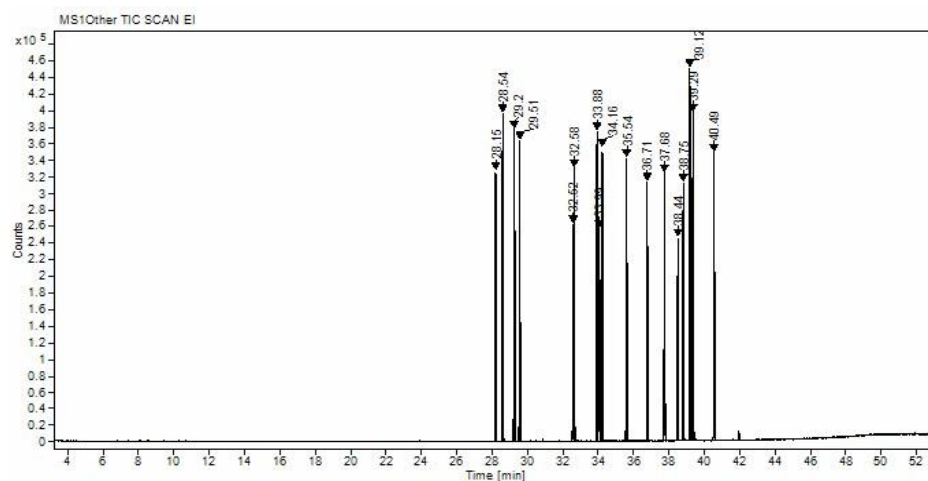

Instrument
GC/MS

Detection
MS

Column
Optima-5MS, 0.25 µm,
0.25 mm

Method Details
Temp: 60°C / 5 min -> 280°C /
6 min, Gradient: 5°C/min

Inj.-Vol.
1.0 µL

Flow
1 mL/min

Method of Preparation

The certified value is based on gravimetric and volumetric preparation of this RM. This RM has been confirmed by the appropriate analytical techniques.

Batch Information

Solvent: Acetonitrile, Lot No. 17057048, 100.00 mL.
Endrin may decompose during GC analysis
to Endrin-aldehyde and Endrin-ketone.

Intended Use

This RM is intended for use in a laboratory as a calibration and quality control standard or in method development for analytical techniques.

Safety

Proper precautions should be observed while handling. See Safety Data Sheet.

Uncertainty

The certified value(s) and uncertainty(ies) are determined in accordance with ISO 17034 with an 95% confidence level ($k=2$). Uncertainty is based on the Total Combined Uncertainty, including uncertainties of preparation, purity of neat materials, homogeneity and stability testing. Stability values are based on real evidence opposed to simulation.

Traceability

The balances used for gravimetric measurements are calibrated with weights traceable to the national standards (DKD). The calibration of the balances is verified daily internally and annually by an external accredited calibration service. Only Class A glassware is used for volumetric measurements.

Homogeneity

Random replicate samples of the final packaged RM have been analysed to prove homogeneity consistent with ISO 17034.

Storage

The RM should be stored in the original sealed bottle at the indicated temperature.

Instructions for Use

The RM should be used shortly after opening to avoid concentration changes due to evaporation. It is recommended to use 1 mL as the minimum sample size and if less material is used, to increase the certified uncertainty by a factor of two for half sample and four for a quarter of sample. If the RM was in a sealed ampoule and storage after opening is necessary, it should be transferred to an amber vial with minimum head space and a Teflon-lined silicon septum. Visit the support section of our website lgcstandards.com for a series of Dr. Ehrenstorfer Tech Tip videos and frequently asked questions.

LGC Labor GmbH
Bgm.-Schlosser-Straße 6A
86199 Augsburg, Germany
T | +49 821 906080
F | +49 821 9060888
E | dr.ehrenstorfer@lgcgroup.com

LGC Labor GmbH is accredited by
DAkkS accreditation numbers
D-RM-19883-01-00 & D-PL-19883-01-00
on ISO 17034:2017 & ISO/IEC 17025:2018

