



Certificate of Analysis

ISO 9001

Reference Material

Product name

trans-Clopenthixol Dihydrochloride

Product code

MM0827.06-0025

CAS number

58045-22-0

Molecular weight

473.89

Molecular formula $C_{22}H_{25}ClN_2OS \cdot 2HCl$ **Lot number**

1013032

Appearance


white solid

Melting point

240 °C (dec)

Long-term storage

2 to 8 °C, dark

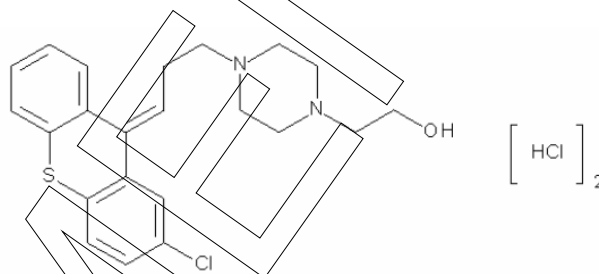Assay "as is"
94.5 %

Date of shipment:

02 Sep 2019

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **one year** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

| | | | |
|---------------------|--------------------------|--|-----------------|
| Release by: | Date of Release: | | Product Release |
| Dr. Sabine Schröder | Luckenwalde, 06 Aug 2019 | | |



MikromolTM

Product information

For laboratory use only. Not suitable for human or animal consumption.

Before usage of the RM, it should be allowed to warm to room temperature. No drying required, as the certified value is already corrected for the content of water and other volatile materials.

The product quality is controlled by regularly performed quality control tests (retests).

Further content

Identity

Assay

Final result

Revision table


SPECIMEN



Identity


The identity of the reference material was established by following analyses.

| Method | Conditions | Result |
|--------------------|---------------------------|---------------------|
| ¹ H-NMR | 400 MHz, D ₂ O | Structure confirmed |

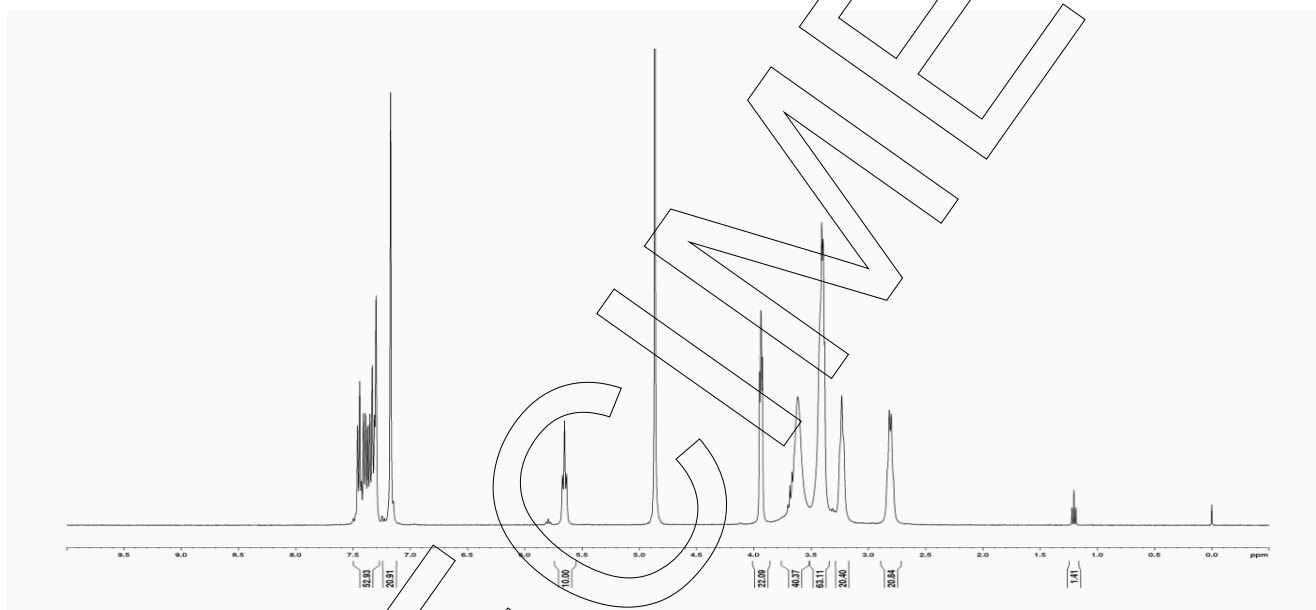




| Method | Conditions | Result |
|--------|--|---------------------|
| MS | 3.5 kV ESI+; capillary temperature: 269 °C Theoretical value: 401.14489 | Structure confirmed |

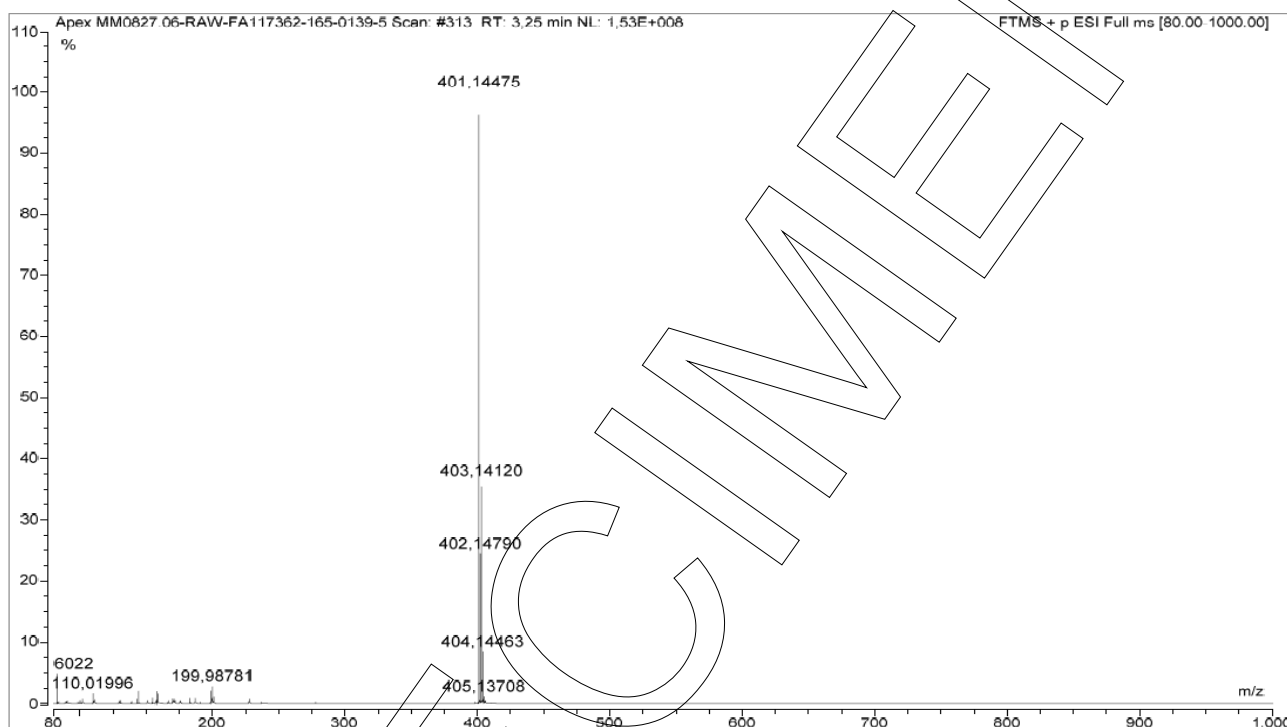



| Method | Conditions | Result |
|--------|--|---------------------|
| IR | Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy | Structure confirmed |

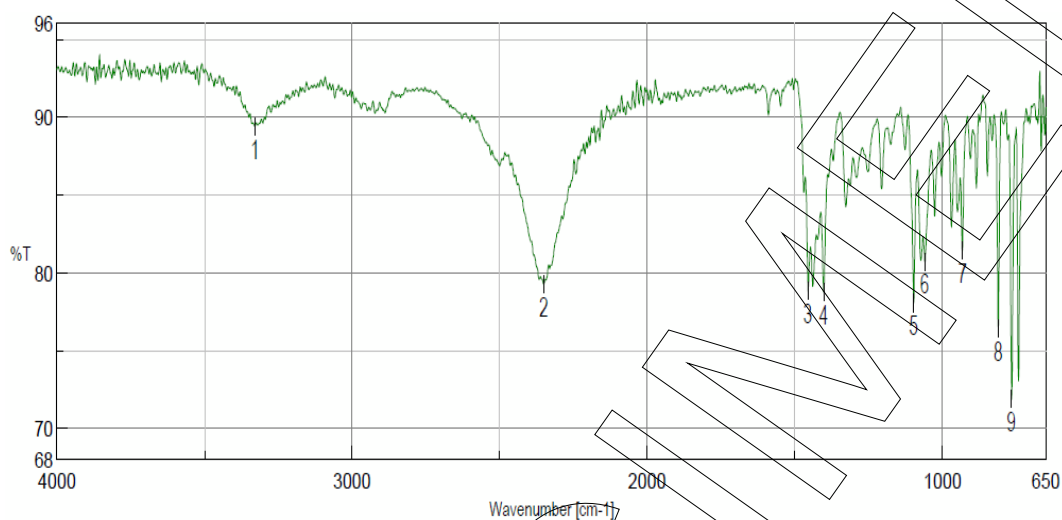

| Results of Peak Find | | |
|----------------------|----------|-----------|
| No. | Position | Intensity |
| 1 | 3329.5 | 89.379 |
| 2 | 2350.8 | 79.238 |
| 3 | 1455.03 | 78.8327 |
| 4 | 1402 | 78.7626 |
| 5 | 1097.3 | 78.0357 |
| 6 | 1059.69 | 80.6868 |
| 7 | 932.414 | 81.4023 |
| 8 | 810.92 | 76.3836 |
| 9 | 765.601 | 71.862 |

Assay


The assay of the reference material was assessed by following analyses.

Purity by High Performance Liquid Chromatography (HPLC)

| HPLC Conditions: | |
|--------------------|--|
| Column | Hypersil Gold C18; 5 µm, 150 x 4.6 mm |
| Column temperature | 40 °C |
| Detector | DAD, 210 nm |
| Injector | Auto 5 µl; 0.103 mg/ml in Water |
| Flow rate | 1.0 ml/min |
| Phase A | Water, 0.1 % H ₃ PO ₄ |
| Phase B | Acetonitrile, 0.1 % H ₃ PO ₄ |
| Gradient program | 0-10 min A/B 70/30 10-13 min A/B to 30/70 13-15 min A/B 30/70 15-18 min A/B to 70/30 18-25 min A/B 70/30 (v/v) |



HPLC chromatogram and peak table

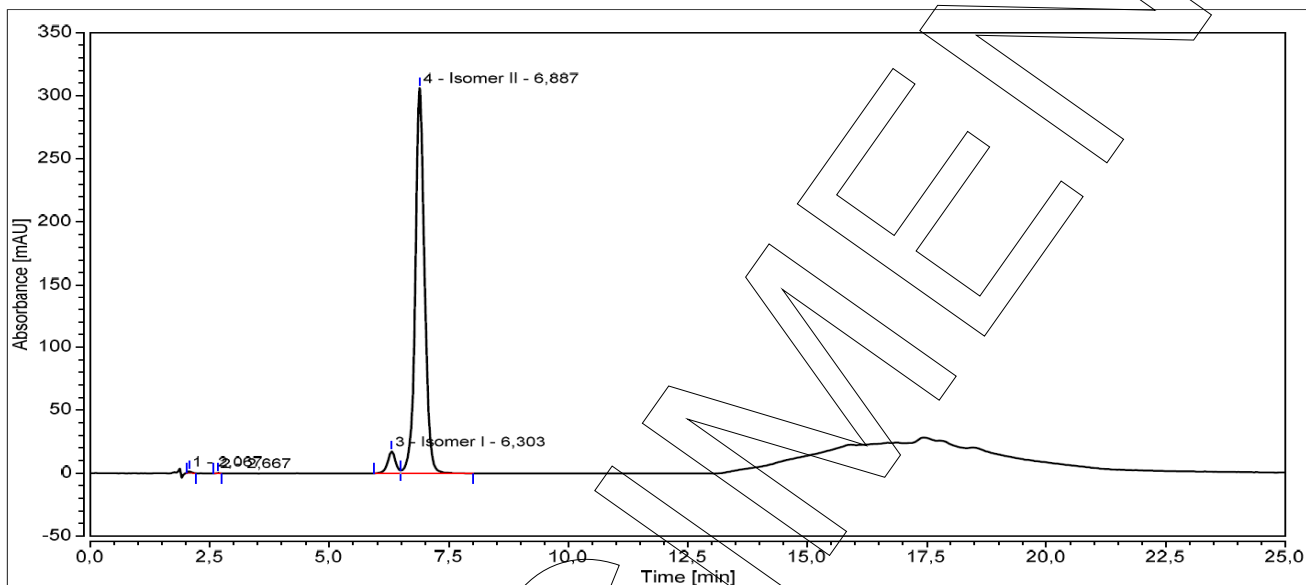

Area percent report - sorted by signal

| Pk # | Retention time | Area | Area % | |
|--------|----------------|--------|--------|--------------|
| 1 | 2.067 | 0.132 | 0.18 | |
| 2 | 2.667 | 0.034 | 0.05 | |
| 3 | 6.303 | 3.375 | 4.66 | cis-Isomer |
| 4 | 6.887 | 68.839 | 95.11 | trans-Isomer |
| Totals | | 72.38 | 100.00 | |

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

Result (n = 3)

95.08 %; SD = 0.03 %



Volatile content

Water content

| | |
|-----------------------|------------------------|
| Method | Karl Fischer titration |
| Result (n = 3) | 0.19 %; SD = 0.01 % |

Residual solvents

| | |
|-----------------------|-------------------------------|
| Method | ¹ H-NMR |
| Result (n = 1) | Sum: 0.45 % 0.45 % Ethanol |

Final result

Assay "as is": 94.47 %

The assay "as is" is assessed by 100% method (mass balance) and is equivalent to the assay based on the not anhydrous and not dried substance respectively.

The calculation of the 100% method follows the formula:

$$\text{Assay (\%)} = (100 \% - \text{volatile contents (\%)}) * \frac{\text{Purity (\%)}}{100 \%}$$

Volatile contents are considered as absolute contributions and purity is considered as relative contribution. Inorganic residues are excluded by additional tests.

Revision table

| Revision | Date | Reason for revision |
|----------|-------------|--|
| 00 | 06 Aug 2019 | Release of the Certificate of Analysis - initial version |

Product warranties for the RM are set out in the terms and conditions of purchase.