

This certificate is designed in accordance with ISO 17034 and ISO Guide 31. This certified reference material (CRM) was designed, produced and verified in accordance with ISO/IEC 17025, ISO 17034 and a registered quality management system ISO 9001.

Certified Reference Material

Product Name
Phthalate Mixture 509 1000 µg/mL in Hexane

Product Code
DRE-A50000509HE

Lot Number
2-H459309HE

Format
Multicomponent Solution

Expiry Date
15 Aug 2026

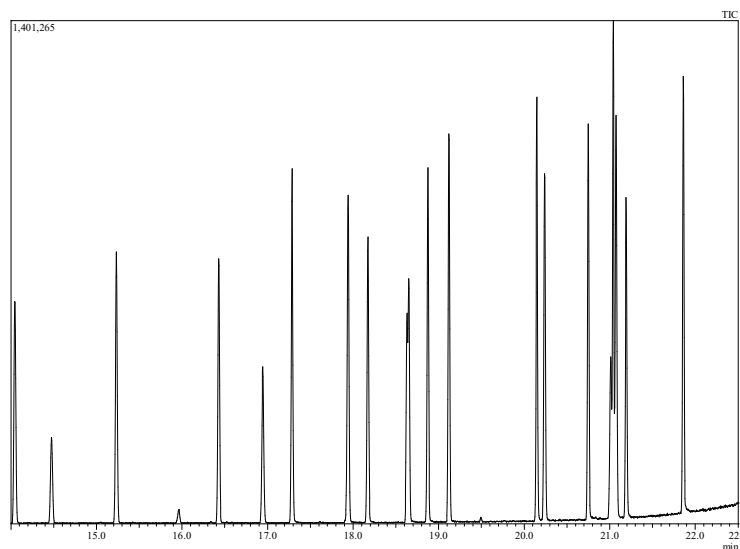
Storage Temp
≤ -10 °C

Compound Name	CERTIFIED		CAS	Lot Number	Purity (%)	Amount (mg)	RT (min)
	Concentration (µg/mL)	Expanded Uncertainty U (µg/mL)					
Di-nonyl Phthalate	993.8	51	84-76-4	3759.34P	99.5	23.97	
Dimethyl Phthalate	1004	51	131-11-3	39.9.2P	99.9	24.12	14.05
Diethyl Phthalate	1004	51	84-66-2	38.7.1P	99.8	24.15	15.23
Diallyl Phthalate	1006	51	131-17-9	3310.7.1P	99.2	24.34	16.43
Di-n-butyl Phthalate	990.4	54	84-74-2	40.9.2P	99.8	23.82	17.29
Diisobutylphthalate	1007	51	84-69-5	1899.7.1.1P	99.2	24.36	17.94
Bis(2-methoxyethyl)phthalate	983.4	53	117-82-8	2254.286.1.1P	98.5	23.96	18.17
Bis(4-methyl-2-pentyl)phthalate	997.4	51	146-50-9	2255.8544.3.1P	99.5	24.06	18.63
Bis(2-ethoxyethyl)phthalate	1008	51	605-54-9	2253.3.13P	98.4	24.59	18.87
Diamyl Phthalate	991.2	50	131-18-0	3058.7.2P	99.4	23.93	19.12
Di-n-hexyl Phthalate	1015	51	84-75-3	2474.7.2P	99.4	24.51	20.15
Butyl Benzyl Phthalate	983.1	53	85-68-7	36.1.5P	98	24.08	20.24
Bis(2-butoxyethyl) Phthalate	985.4	51	117-83-9	2252.3.12P	97.8	24.18	20.75
Bis(2-ethylhexyl)phthalate	1006	55	117-81-7	33.29.1P	99.4	24.29	21.04
Dicyclohexyl Phthalate	997	50	84-61-7	2171.7.2P	99.9	23.95	21.07
Diphenyl Phthalate	986.4	54	84-62-8	3479.1.1P	98.6	24.01	21.19
Di-n-octyl Phthalate	986.2	50	117-84-0	41.7.5P	99.1	23.88	21.86

The producer certifies that this reference material meets the specification stated in this certificate until the expiry date, provided it is stored unopened at the recommended temperature herein. Product warranties for this reference material are set out in the terms and conditions of purchase.

CERTIFIED BY	CERTIFIED ON		RM Release

CHROMATOGRAM

Instrument
GC/MSDetection
MSColumn/Flow
Phenomenex ZB-Semivolatle 30m
x 0.25 mm, ID 0.25 um / 1 mL/min

Method Details		
Rate Temp.(C)	Hold time (min)	
40.0	2.0	
10.0	100.0	0.0
15.0	250.0	0.0
20.0	345.0	3.25

Inj.-Vol
1 µL**Method of Preparation**

The certified value is based on gravimetric and volumetric preparation of this CRM. This CRM has been confirmed by the appropriate analytical techniques.

Batch Information

Solvent: Hexane, Lot no. 204550, 24 mL

Intended Use

This CRM is intended for use in a laboratory as a calibration and quality control standard or in method development for analytical techniques.

Safety

Proper precautions should be observed while handling. See Safety Data Sheet.

Uncertainty

The certified value(s) and uncertainty(ies) are determined in accordance with ISO 17034 with an 95% confidence level (k=2). Uncertainty is based on the Total Combined Uncertainty, including uncertainties of preparation, purity of neat materials, homogeneity, long-term stability testing, and transportation stability.

Traceability

The balances used for gravimetric measurements are calibrated with weights traceable to the national standards (NIST). The calibration of the balances is verified daily internally and annually by an external accredited calibration service. Only Class A glassware is used for volumetric measurements.

Homogeneity

Random replicate samples of the final packaged CRM have been analysed to prove homogeneity consistent with ISO 17034.

Storage

The CRM should be stored in the original sealed bottle at the indicated temperature.

Instructions for Use

The CRM should be used shortly after opening to avoid concentration changes due to evaporation. It is recommended to use 1 µL as the minimum sample size. If storage after opening is necessary, it should be transferred to an amber vial with minimum head space and a Teflon lined silicon septum. If handled as recommended, use period after opening is a maximum of 437 days for an estimated 5% drift in concentration as a result of analyte and/or solvent transpiration. Visit the support section of our website lgcstandards.com for a series of Dr. Ehrenstorfer Tech Tip videos and frequently asked questions.

LGC Group
7290-B Investment Drive
North Charleston, SC 29418
United States
T | +1 843 763 4884
F | +1 866 509 5146
E | dr.ehrenstorfer@lgcgroup.com

The producer of this reference material is registered to ISO 9001:2015 under 56 100 19560019 by TUV USA and accredited to ISO 17025:2017 and ISO 17034:2016 by A2LA with the accreditation numbers 3031.01 and 3031.02.



ISO 17034 Accredited
Reference Material Producer
Cert. No. 3031.02