

Certificate of Analysis

ISO 9001

Reference Material

Product name

1-Methyl-12-thioxopyrido[1',2':3,4]imidazo-[1,2-a]benzimidazol-2(12H)-one

Product code

MM0474.13-0025

CAS number

1246819-06-6

Molecular weight

267.31

Molecular formula

C₁₄H₉N₃OS

Lot number

1186870

Appearance


red solid

Melting point

222 °C

Long-term storage

2 to 8 °C, dark

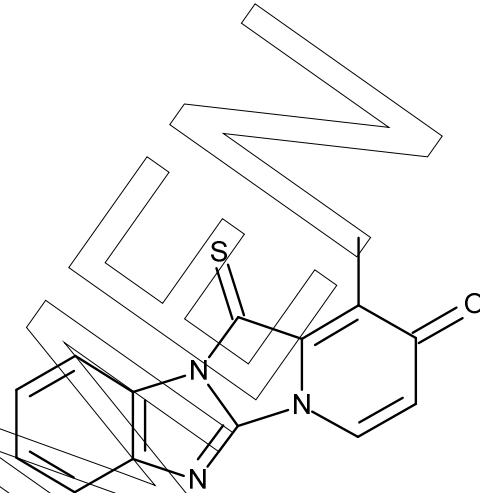

Assay "as is"
99.1 %

Date of shipment:

08 Nov 2021

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **two years** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

Release by:	Date of Release:		Product Release
Dr. Sabine Schröder	Luckenwalde, 20 Oct 2021		



Product information

For laboratory use only. Not suitable for human or animal consumption.

Before usage of the RM, it should be allowed to warm to room temperature. No drying required, as the certified value is already corrected for the content of water and other volatile materials.

The product quality is controlled by regularly performed quality control tests (retests).

Further content

Identity

Assay

Final result

Revision table


SPECIMEN



Identity

The identity of the reference material was established by following analyses.

Method	Conditions	Result
¹ H-NMR	400 MHz, CDCl ₃	Structure confirmed

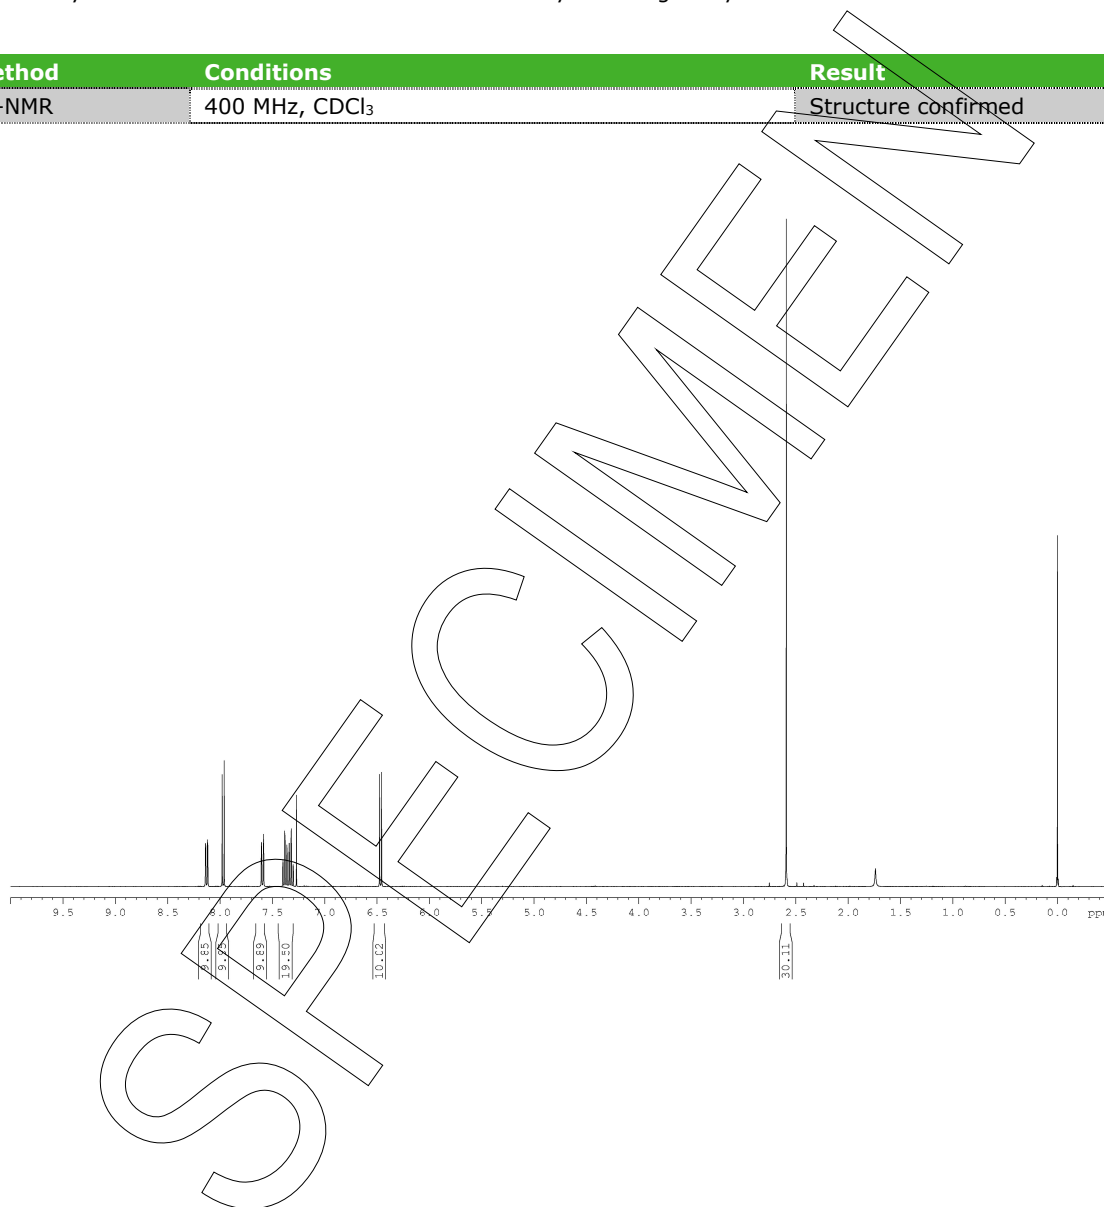




Assay

The assay of the reference material was assessed by following analyses.

Purity by High Performance Liquid Chromatography (HPLC)

HPLC conditions:	
Column	LiChrospher 60 RP-select B; 5 µm, 125 x 4 mm
Column temperature	40 °C
Detector	DAD, 280 nm
Injector	Auto 6 µl; 0.050 mg/ml in Acetonitrile
Flow rate	1.0 ml/min
Phase A	Water, 0.1 % H ₃ PO ₄
Phase B	Acetonitrile, 0.1 % H ₃ PO ₄
Gradient program	0-12 min A/B 65/35 12-25 min A/B to 30/70 25-30 min A/B 30/70 30-35 min A/B to 65/35 35-40 min A/B 65/35 (v/v)

HPLC chromatogram and peak table

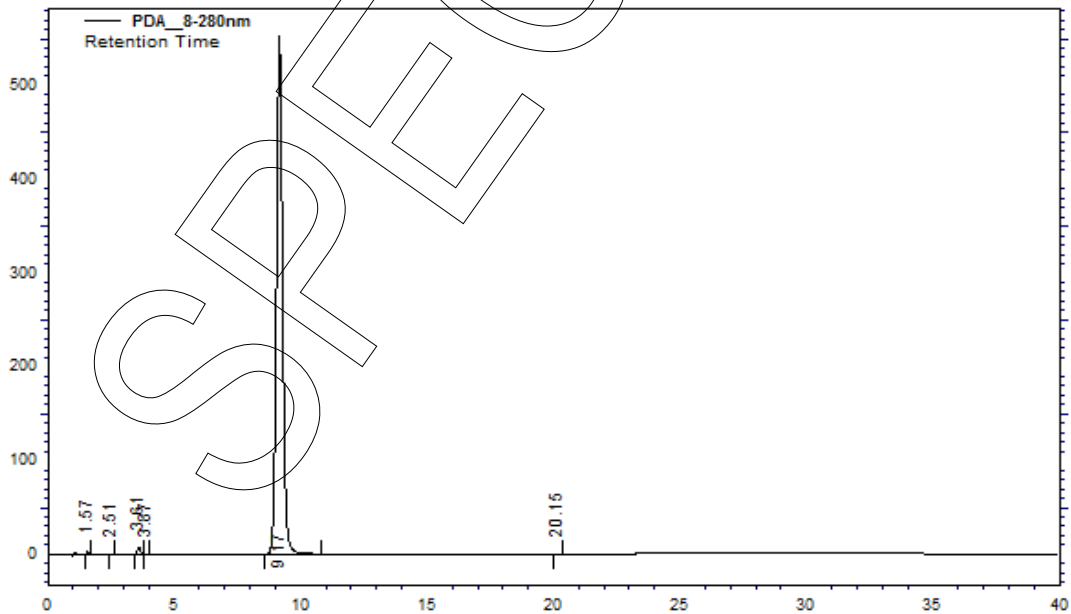



Area percent report - sorted by signal

Pk #	Retention time	Area	Area %
1	1.57	13793	0.15
2	2.51	2390	0.03
3	3.61	52755	0.58
4	3.87	4183	0.05
5	9.17	9044316	99.19
6	20.15	1189	0.01
Totals		9118626	100.00

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

Result (n = 6) 99.18 %; SD = 0.03 %

Volatile content

Loss on drying

Method TGA
Result 0.05 %



Final result

Assay "as is": 99.13 %

The assay "as is" is assessed by 100% method (mass balance) and is equivalent to the assay based on the not anhydrous and not dried substance respectively.

The calculation of the 100% method follows the formula:

$$\text{Assay (\%)} = (100 \% - \text{volatile contents (\%)}) * \frac{\text{Purity (\%)}}{100 \%}$$

Volatile contents are considered as absolute contributions and purity is considered as relative contribution. Inorganic residues are excluded by additional tests.

Revision table

Revision	Date	Reason for revision
00	20 Oct 2021	Release of the Certificate of Analysis – initial version

Product warranties for the RM are set out in the terms and conditions of purchase.