




Mikromol™

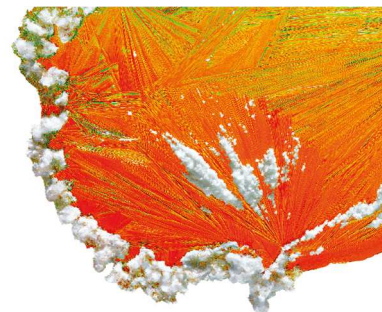

Certificate of Analysis

ISO 17034

Reference Material

Product name

Prednisone Acetate

Product code

MM0196.00

CAS number

125-10-0

Molecular weight

400.46

Molecular formula

C₂₃H₂₈O₆

Lot number

G1013706

Appearance


white solid

Melting point (DSC)

237 °C

Long-term storage

2 to 8 °C, dark

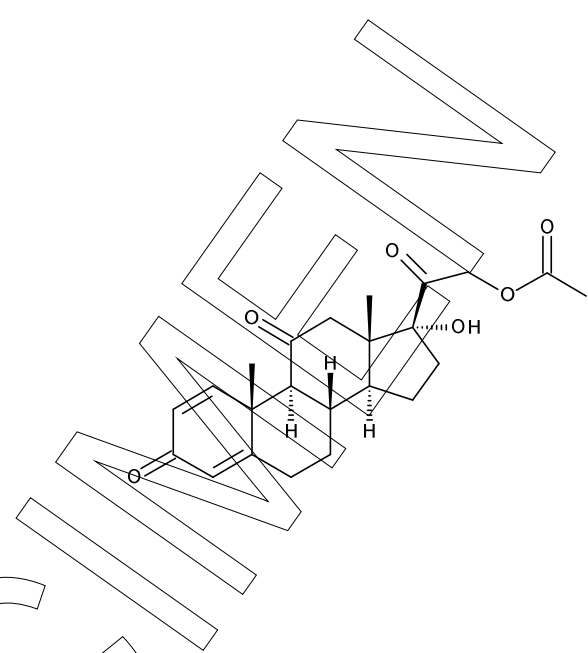

Assay¹ "as is"
97.5 %

Uncertainty² U
0.4 %

Intended Use: Use for identification and quantification. The assay is verified by a second testing method. Due to the homogeneity studies, the minimum amount of sample to be used is 10 mg.

Date of shipment: **01 Sep 2020**

Producer confirms that this reference material (RM) meets the specification detailed on this Certificate of Analysis for **two years** from the date of shipment, provided the substance is stored under the recommended conditions unopened in the original container.

Release by:	Date of Release:		Product Release
Dr. Sabine Schröder	Luckenwalde, 10 Aug 2020		

¹ Calibration and verification were carried out using standards traceable to SI-units. The value is expressed on an "as is" basis.

² The uncertainty "U" is the expanded uncertainty of the testing method for the assigned value estimated in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM). It corresponds to a level of confidence of about 95%. Coverage factor k = 2.



Important product information

This RM is intended for laboratory use only and is not suitable for human or animal consumption.

This RM conforms to the characteristics of a primary standard as described in the ICH Guidelines. The values quoted in this Certificate of Analysis are the producer's best estimate of the true values within the stated uncertainties and based on the techniques described in this Certificate of Analysis. The production of this RM was undertaken in accordance with the requirements of ISO 17034. The identity is verified by data from international scientific literature.

Storage and handling

Before usage of the RM, it should be allowed to warm to room temperature. No drying is required, as assigned values are already corrected for the content of water and other volatile materials.

Further content

Assigned value

Purity

Identity

Stability and homogeneity

Revision table



Assigned value

Assay "as is": 97.50 %; U = 0.37 %

The assay "as is" is assessed by 100% method (mass balance) and is equivalent to the assay based on the not-anhydrous and not-dried substance. The assay is verified by quantitative NMR spectroscopy. The verified result lies inside our acceptance criteria, i.e. less than 1.0 % difference to assay assigning technique.

For quantitative applications, use the assay as a calculation value on the "as is basis". The uncertainty of the assay can be used for estimation/calculation of measurement uncertainty.

Method 1: Value assigning technique - 100% method

100% method (mass balance) with chromatographic purity by HPLC

Result

97.50 %; U = 0.37 %

The calculation of the 100% method follows the formula:

$$\text{Assay (\%)} = (100 \% - \text{volatile contents (\%)}) * \frac{\text{Purity (\%)}}{100 \%}$$

Volatile contents are considered as absolute contributions and purity is considered as relative contribution. Inorganic residues are excluded by additional tests.



Method 2: Value verifying technique - quantitative NMR spectroscopy

Conditions

400 MHz, CDCl₃


Internal standard

Methyl 3,5-dinitrobenzoate (certified reference material), signal 8.7 – 9.7 ppm, 3 H

Result (mass fraction, n = 6)

98.18 %

Quantitative NMR spectrum

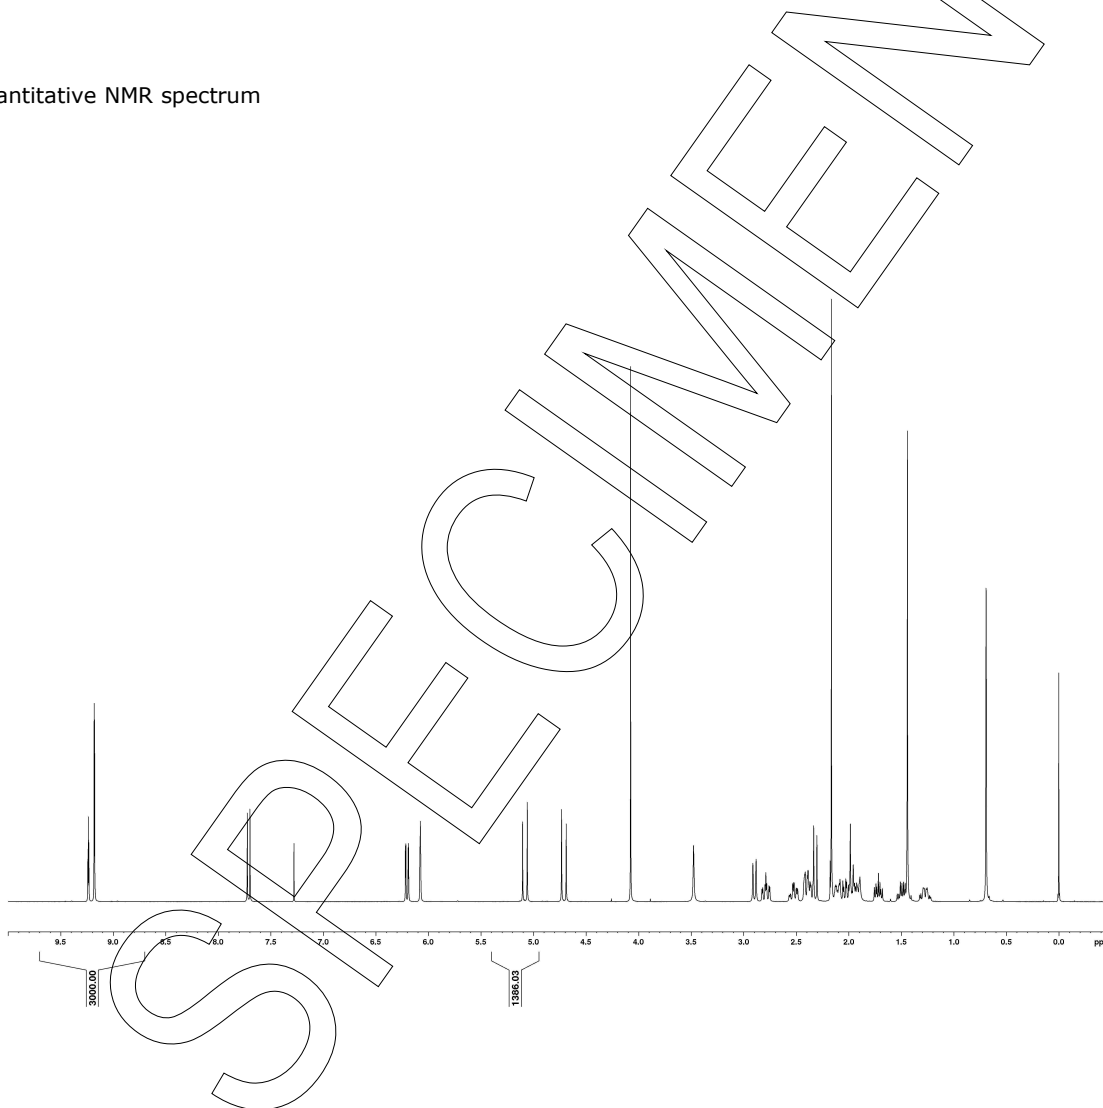




Purity

Purity by High Performance Liquid Chromatography (HPLC)

HPLC conditions:	
Column	Hypersil Gold C18; 5 µm, 150 x 4.6 mm
Column temperature	40 °C
Detector	DAD, 240 nm
Injector	Auto 5 µl; 0.151 mg/ml in Water/Acetonitrile 50/50 (v/v)
Flow rate	1.0 ml/min
Phase A	Water, 0.1 % H ₃ PO ₄
Phase B	Acetonitrile, 0.1 % H ₃ PO ₄
Gradient program	0-20 min A/B 70/30 20-25 min A/B to 20/80 25-30 min A/B 20/80 30-33 min A/B to 70/30 33-40 min A/B 70/30 (v/v)

HPLC chromatogram and peak table

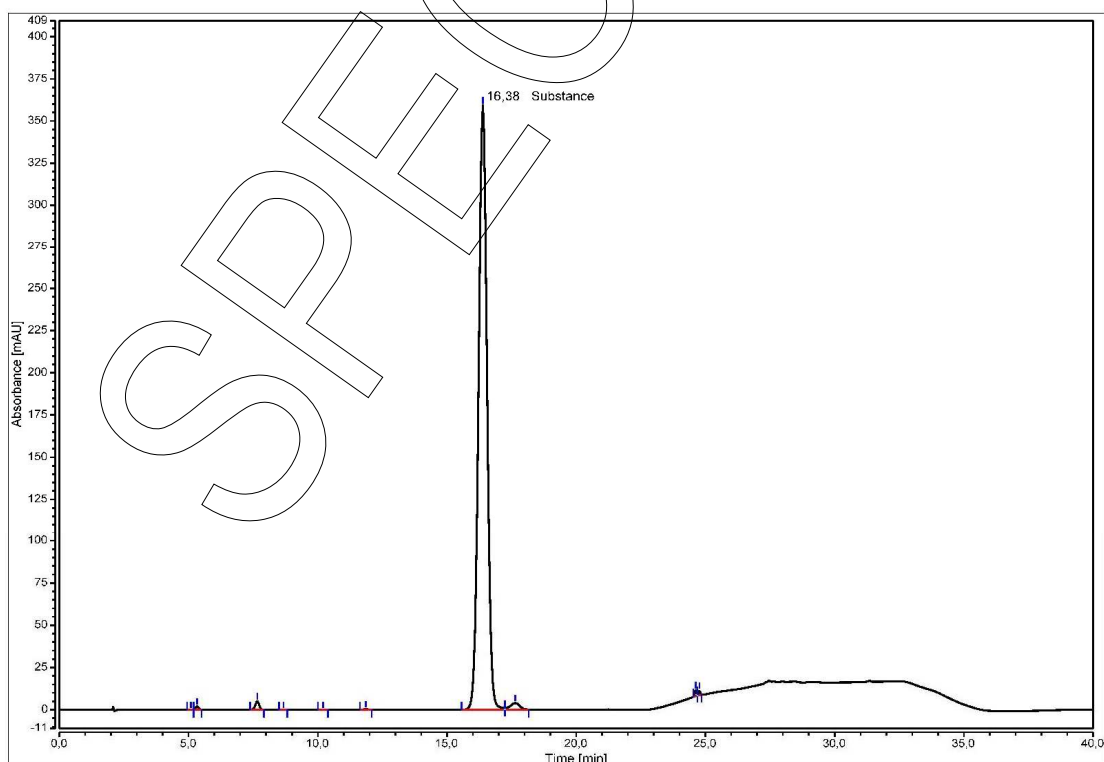



Area percent report - sorted by signal

Pk #	Retention time	Area	Area %
1	5.083	0.012	0.01
2	5.333	0.259	0.19
3	7.657	0.892	0.64
4	8.678	0.010	0.01
5	10.210	0.026	0.02
6	11.862	0.065	0.05
7	16.383	135.271	97.49
8	17.640	1.679	1.21
9	24.622	0.307	0.22
10	24.763	0.229	0.16
Totals		138.749	100.00

The content of the analyte was determined as ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100 %. System peaks were ignored in calculation.

Result (n = 10) 97.50 %; U = 0.37 %

Volatile content

Water content

Method Karl Fischer titration

Result (n = 3) No significant amounts of water were detected (< 0.05 %).*

* not accredited testing method

Residual solvents

Method GC headspace

Result (n = 3) No significant amounts of residual solvents were detected (< 0.05 %).



Inorganic residues

Method: Sulphated ash*, EP 8.7 (2.4.14)


According to the available data, the presence of inorganic impurities in the reference material other than those detectable by sulphated ash is highly unlikely. Inorganic residues can be excluded by results of the sulphated ash. Therefore, no assay correction was performed for inorganic impurities.

* not accredited testing method

Identity


The identity is assessed by ISO/IEC 17025 accredited testing methods.

Method	Conditions	Result
¹ H-NMR	400 MHz, CDCl ₃	Structure confirmed

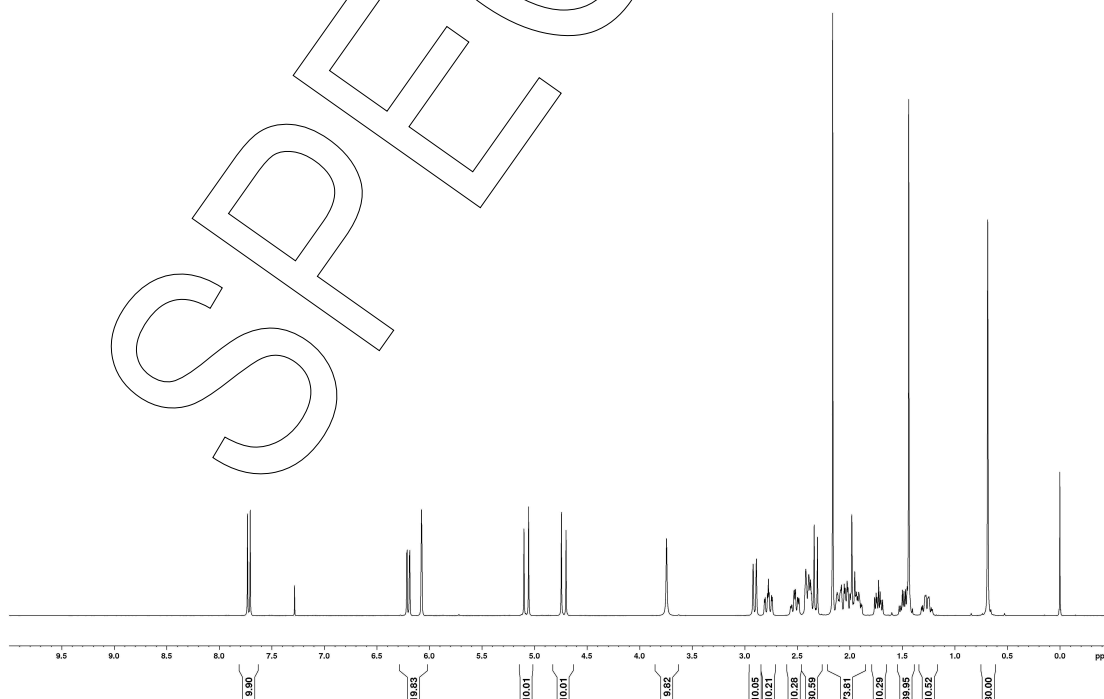




Method	Conditions	Result
MS	3.5 kV ESI+; capillary temperature: 269 °C Theoretical value: 401.19587	Structure confirmed

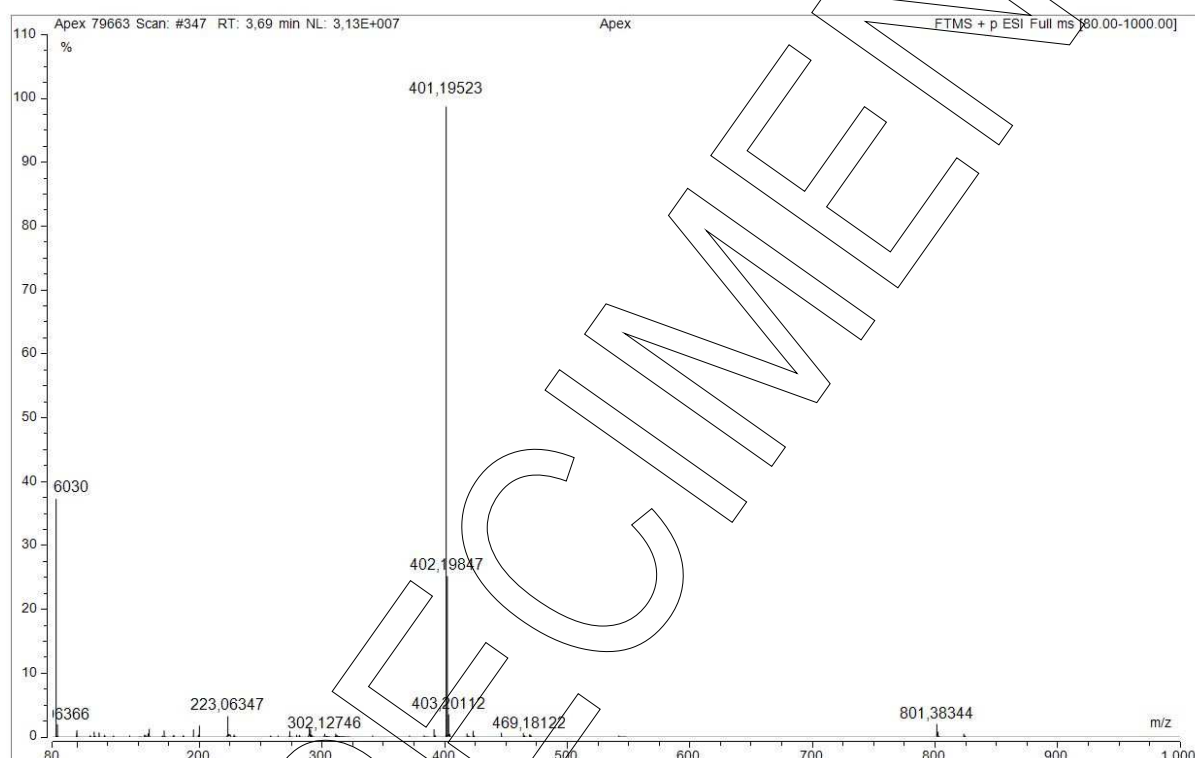



Method	Conditions	Result
IR	Attenuated Total Reflection Fourier Transform Infrared (ATR-FTIR) Spectroscopy	Structure confirmed

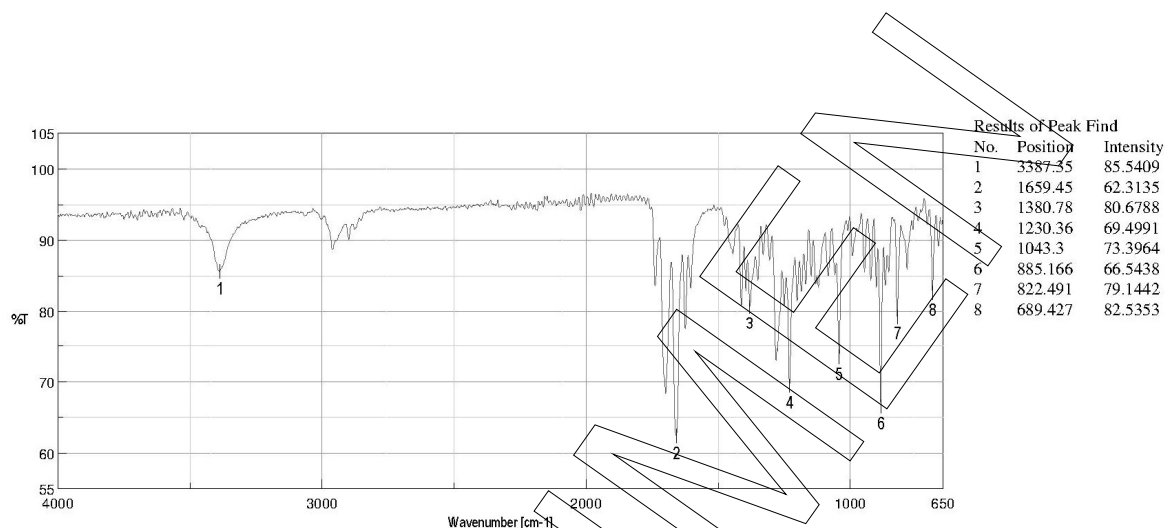

Stability and homogeneity

The assessment of stability indicates no significant instability. The given validity period is based on this data. This is backed up by additional stability testing and historical data over the range of several years.

RM quality is controlled by regularly performed quality control tests (re tests). Homogeneity assured by qualified process of preparation and verified by homogeneity testing.

Revision table

Revision	Date	Reason for revision
00	14 Aug 2020	Release of the Certificate of Analysis - initial version

Product warranties for the RM are set out in the terms and conditions of purchase.